

UNCLASSIFIED

AD NUMBER
AD836238
NEW LIMITATION CHANGE
TO Approved for public release, distribution unlimited
FROM Distribution authorized to U.S. Gov't. agencies and their contractors; Critical Technology; JUN 1965. Other requests shall be referred to Department of the Army, Fort Detrick, Attn: Technical Release Branch/TID, Frederick, MD 21701.
AUTHORITY
SMUFD D/A ltr, 14 Feb 1972

THIS PAGE IS UNCLASSIFIED

AD 836238

TRANSLATION NO. 1437

DATE: JUNE 1965

DDC AVAILABILITY NOTICE

Reproduction of this publication in whole or in part is prohibited. However, DDC is authorized to reproduce the publication for United States Government purposes.

STATEMENT #2 UNCLASSIFIED

This document is subject to special export controls and each transmittal to foreign governments or foreign nationals may be made only with prior approval of Dept. of Army, Fort Detrick, ATTN: Technical Release Branch/TID, Frederick, Maryland 21701

DEPARTMENT OF THE ARMY  
Fort Detrick  
Frederick, Maryland

*Anal. Assoc. Química Argentina 51(1):  
96-122, 1963*

## EVALUATION OF MICRO QUANTITIES OF ALUMINUM

by

Julia Flavia Possidoni de Albinati

**SUMMARY** -- A study was made of the fluorometric procedure used for the determination of microquantities of Aluminum based on the reaction with Pontachrome blue-black-R. Although several papers were written on this subject, lack of agreement was found specially on the influence of certain elements. The operating conditions of the Beckman spectral fluorescence attachment were established, and fluorescent spectra of both reagent and aluminum compound obtained. The optimum wave length for aluminum determination was 605 m $\mu$ . The influence of pH, solvent and concentration of the reagent, time of heating, fluorescence stability, etc., were studied and a sensitivity of 0.0001  $\gamma$  Al/ml was attained. The effect of about 70 different ions was considered and in a next paper a method for the elimination of interference will be discussed.

### INTRODUCTION

The ideal analytical identification and evaluation of a given ion in the presence of any other by the use of reagents has not been carried out yet. On the other hand, new and more selective agents have been incorporated repeatedly for analytical purposes. However, when the analysis is associated with unfavorable relations as far as the evaluation of the ion is concerned, namely with interference, the solution becomes more and more complicated.

The purpose of this experiment is to develop a relatively simple process to obtain correct data in the evaluation of micro quantities of aluminum when this ion is in the presence of much larger quantities of any other ion.

For this purpose, the Pontachrome blue-black-R [See note] was used, since it is a reagent which permits the achievement of great sensitivity and, according to the bibliographical information which will be analyzed later, would experience relatively few interferences.

[Note:] Also known as Superchrome-blue-black, Blue au chrome 2R, Blue noir au chrome NR, Blue noir solochrome BS, and appears with the number 202 in the Color Index (CI 202). In this paper we will use the abbreviation CI 202.

In 1937 White and Lowe (1) described for the first time the use of CI 202 as reagent for aluminum. This compound is the sodium salt of the acid 4-sulfo 2-2 dehydroxy-azo-naphtalene. In that paper it was stated that the orange fluorescence characteristic of the complex that aluminum forms with this reagent could experience interference only by certain colored ions and by the fluoride ion, and it was specially recommended for the evaluation of aluminum in the presence of berilium. The influence of acids and alkalis on fluorescence was also indicated. Gallium was included among the ions which would not interfere. The sensitivity attained using a mercury lamp as source was 1:5,000,000 (using a 0.1% solution of the reagent).

Later on, in 1941, Bourstyn (2) studied this coloring agent again, mentioning the previous paper and stating the importance of provoking the reaction at the pH at which aluminum hydroxide precipitates. The sodic salt of the reagent was used in a 1% alcoholic solution, and the pH was controlled using an acetate-acetic solution. The author attained a sensitivity of  $2 \times 10^{-4}N$ , which decreases when the fluoride ion is eliminated with boric acid.

In 1944 Weissler and White (3) developed a method for the determination of aluminum in steel, bronze and minerals based on the use of CI 202. In that experiment they studied the influence of pH, time, heating and concentration of the reagent. Interferences were eliminated by electrolysis using a mercury cathode. They also analyzed the fluorescent compound, obtaining a relation Al:CI 202 = 1:2. The sensitivity attained with this method was 1:125,000,000.

Later on, in 1947, Charlot (4) after studying several reagents for the ions of the aluminum group, indicated that CI 202 is one of the most convenient ones. This author worked with an aqueous solution of the reagent (0.01%) and controlled pH with an acetic-acetate solution. The sensitivity attained with the proposed semi-quantitative technique was 0.01  $\gamma$  of Aluminum per ml. (1:100,000,000). Among the interfering ions the author mentions:

Chrome (III) and uranium (VI): interfere slightly.  
Cobalt (II) and molybdenum (VI): interfere considerably.  
Mickel (II), copper (II), iron (III), titanium (IV), vanadium (IV) and vanadium (V): stop the reaction.

Iron (II): undesirable because it oxidizes forming iron (III).  
Cerium (IV), thallium (III), gold (III) and platinum (IV): oxidize  
the coloring agent.  
Chromium (IV): undesirable because of its color.  
Oxalates and fluorides: must be eliminated before the reaction.  
Galium (III): interferes.

Separations are indicated by extracting the cupferrates in ethyl acetate (galium, iron, etc.) or by precipitation and filtration (gold, platinum). To eliminate the interference of cobalt, nickel and copper, the formation of a complex of these ions with cyanide is provoked.

In 1957 Ishibashi and his associates (5) made a new study of the application of CI 202 to the evaluation of aluminum. After studying the influence of pH, they considered convenient to provoke the reaction at pH 4.8. To develop fluorescence they heated the solution in a double boiler for ten minutes. They suggest adding different volumes of 0.1% alcoholic solution, according to the amount of aluminum present [See note]. With the proposed method they detected 0.004  $\gamma$  of aluminum per milliliter. In this paper they studied the effects of several ions, fifteen of them, and established that  $\text{Ca}^{++}$ ,  $\text{Mg}^{++}$ ,  $\text{Sr}^{++}$ ,  $\text{Ba}^{++}$ ,  $\text{In}^{+++}$ ,  $\text{Mn}^{++}$ ,  $\text{F}^-$  and  $\text{PO}_4^{3-}$  do not interfere with the reaction.  $\text{Cu}^{++}$ ,  $\text{Ti}^{4+}$  and  $\text{Ni}^{++}$  would produce negative errors. Greater negative errors would be obtained with  $\text{Co}^{++}$  and  $\text{VO}_3^-$ .  $\text{Fe}^{+++}$  should not be present, and its reduction to  $\text{Fe}^{++}$  using hydroxylamine would not eliminate its interference completely.  $\text{Ga}^{+++}$  produces positive errors because of its fluorescence. The fact that in considering the influence of the different ions the authors have not attained ratios of Al: interference better than 1:20 (except for  $\text{Mg}^{++}$ , where Al:Mg = 1:500) [See note 2] should be taken into consideration.

[Note 1] In the summary of the original paper the use of 1% aqueous solution of the coloring agent is mentioned, although when referring to reagents and apparatus, (cap. 2) a 0.1% solution in alcohol is prepared.

[Note 2] It is convenient to mention that in the summary of this paper; C. A. 15.333g (1958) it is mentioned that: "Co<sup>++</sup>, VO<sub>3</sub><sup>-</sup> and large quantities of Cu, Ti and Ni do not interfere," while in the original paper it is stated that "the elements Fe<sup>+++</sup>, Ca, Co and vanadic acid interfere in the determination of aluminum by this method. Besides, the presence of large quantities of copper, Ti and Ni has a perturbing influence."

Contradictions can be found in the summary of the bibliographic information. Specially important from the analytical point of view are those related to interference and operating conditions. Therefore, it was considered convenient:

I. To study the instrumental modifications which would make possible the success of the method.

II. To review the most important variables in the analytical process with the purpose of developing a technique which would permit the achievement of a high degree of sensitivity and the acquisition of reproducible data.

III. To determine the influence of several ions.

IV. To develop fast methods for the elimination of interference.

In the first part of this paper it is described how the first three goals mentioned above were attained.

#### EXPERIMENTAL PART

##### A. Apparatus and Reagents:

- a) Spectrophotometer Beckman, model DU, provided with:
  - 1) attachment for the determination of spectral fluorescence No. 22850, with mercury lamp No. 2260 and Corning filter No. 9863.
  - 2) attachment for the determination of total fluorescence No. 2980.
  - 3) normal equipment for absorptiometry in the ultraviolet and visible range.
- b) Beckman pH-meter, Zeromatic model.
- c) Controlled pipettes and matrasses.
- d) Silica precipitation glasses.
- e) Silica distillation apparatus with polished junctions.
- f) Drugs: salts, acids, solvents, etc., of good quality "for analysis" or "spectroscopically pure."
- g) The CI 202 used was kindly given by the Duperial company.

##### B. Solutions

In every case deionised water obtained with a "DESTILIT" mixed bed demineralizer was used.

All the solutions prepared for this experiment were preserved in a polythene container, to avoid possible contaminations with aluminum from glass (specially in case of acid solutions).

1) Pattern solutions of aluminum chloride: approximately 900 mg. of  $\text{Cl}_3\text{Al}\cdot 6\text{H}_2\text{O}$  were weighed and the volume was increased to 100 ml. with HCl 1:20. The concentration was evaluated gravimetrically and adjusted to 1,000 mg of aluminum per ml.

2) Standard aluminum solutions (like chloride): these solutions were prepared using the solution obtained in (1), by diluting it in hydrochloric acid of adequate concentration for every specific case.

3) Aluminum nitrate solution: Approximately 1.4 g of  $(\text{NO}_3)_3\text{Al}\cdot 9\text{H}_2\text{O}$  were weighed and its volume changed to 100 ml. using de-ionized water. The concentration was adjusted gravimetrically to 1,000 mg. of aluminum per ml.

4) Standard solutions of aluminum (like nitrate): these were prepared by diluting the solution obtained in (3).

5) Pattern solutions of the different ions: these were prepared with the salts, acids or oxides (conveniently dissolved) which will be mentioned in every case, and the drugs were used in the quantities necessary to obtain concentrations of 100 mg. of element per ml. of solution.

6) Standard solutions of the different ions: these were obtained by diluting the above mentioned solutions.

7) 0.1 and 0.01% solutions of CI 202 in deionized water.

8) 0.1% solution of CI 202 in ethyl alcohol.

9) Controlling acetic-acetate solution: 1M in sodium acetate and acetic acid.

10) Hydrochloric acid solutions: obtained by distilling 50% diluted hydrochloric acid at atmospheric pressure in a quartz distillation apparatus.

11) Sodium hydroxide solution with concentration of approximately 40%: The small particles of sodium hydroxide were washed by decantation at atmospheric pressure in a platinum container using deionized water, and were then dissolved in the same container. The solution was diluted using a convenient volume of deionized water.

12) Less concentrated solutions of hydrochloric acid and sodium hydroxide: These were prepared by diluting the solutions described in (10) and (11) respectively.

### C. Control of the Instrumental Variables:

While trying to attain our first goal, it was taken into account that the last step in the analytic process is the measurement of the fluorescent intensity of the complex formed. These measurements were carried out using the attachment for spectral fluorescence of the Beckman spectrometer, model DU, which permits the reading of fluorescent radiation of a definite wave length. This attachment was preferred to that of total fluorescence because:

a) The tungsten lamp used in the latter is a less powerful excitation source than the mercury lamp used in the spectral fluorescence attachment, therefore, the values of fluorescence intensity -  $I_f$  - obtained were smaller, decreasing the sensitivity of the method.

b) The possibility of choosing the most convenient wave length to carry out the measurement could eliminate the potential influence of fluorescent compounds having different spectrum.

Since the  $I_f$  is measured using an arbitrary scale, the values obtained will vary as soon as the response of the measuring instrument is altered by modifying its sensitivity, the number of diodes connected to the photomultiplier tube, or the slit width.

The correct handling of these variables leads to good analytic results and permits to vary the effectiveness of the method according to the circumstances. Using standard fluorescent glass in the lower part of the container holder, a series of experiments were performed to decide under what conditions the measurements of  $I_f$  may be carried out more conveniently.

1) Reproducibility: Once the instrument was set to work it was observed that the  $I_f$  obtained during a relatively long period of time vary, until they are sensibly different when they become more and more spaced in time. However, taking into account that each reading requires approximately 10 to 15 seconds, a series of more than ten standard solutions may be measured without detecting any influence of this factor. With every series of measurements made in no more than 10 minutes, values for different fluorescence intensities were obtained.

2) Sensitivity control: The sensitivity of the instrument may be increased 8 to 9 times by turning the corresponding dial clockwise from one end to the other [See note]. With the dial in the last position maximum sensitivity is obtained. However, the values of  $I_f$  obtained under this condition are not easily reproducible, and it is necessary to take several readings of every desired intensity. Most of the time it will be sufficient to set the dial between its midpoint and one or two turns before attaining maximum sensitivity.



[Note:] The result is similar to that obtained when measuring flame intensities with this instrument, equipped with the corresponding attachment.

TABLE I  
Reproducibility

Serie N°	I <sub>i</sub>	Average	s	σ	$S = \frac{\sqrt{\sum s^2}}{n-1}$
1	39.5	39.5	0	0	0.00
	39.5		0	0	
	39.4		0.1	0.01	
	39.5		0	0	
	39.6		0.1	0.01	
	39.5		0	0	
2	10.0	10.03	0.03	0.0009	0.05
	10.1		0.07	0.0049	
	10.1		0.07	0.0049	
	9.9		0.13	0.0169	
	10.0		0.03	0.0009	
	10.1		0.07	0.0049	

3) Response of the photomultiplier tube: The response of this sensible element depends on the number of diodes connected. For the measurement of small luminous intensities, like the ones to be measured, it is convenient to operate at large amplifications, although the fluctuations observed in the galvanometer when all the diodes are connected may require several readings, in order to take an average. (Fig. 1).


By connecting nine diodes, sufficiently stable and reproducible values may be obtained, and a good degree of sensitivity is attained.

4) Slit width: It is necessary to take into account that even using maximum amplification for the responses, it is impossible to measure radiation of very small slit width, because the fluorescence intensities to be measured are relatively weak. However, working with slits of the order of 0.5 mm, it will be possible to measure radiation whose band width for medium intensity is approximately 17 mμ using wave lengths of about 600 mμ, which permits good selectivity. It is convenient to point out that if it is not necessary to eliminate radiations of fluorescent interferences with different spectra, the slit width may increase, since the value of the readings increase as a function of the slit width. (Fig. 2).



Fig. 1. Response of the photomultiplier tube.

Fig. 2. Influence of the slit width.

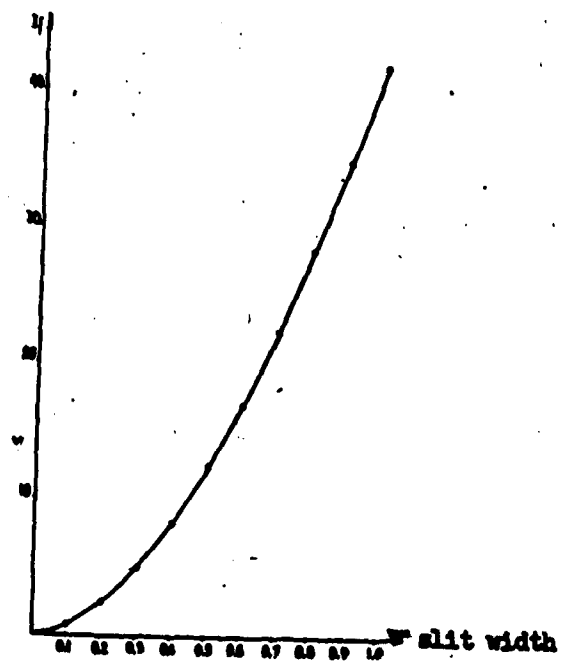

D. Absorption and Fluorescence Spectra:

The absorption spectra corresponding to the reagent and to the complex it forms with aluminum were obtained by preparing a white and a standard in the following form: to 15 ml. of the solution - white or standard - 5 ml. of the acetic-acetate solution and 5 ml. of the 0.01% solution of CI 202 in water were added. This was heated in a double boiler, cooled and used for readings in quartz containers with a light path of 10,000 mm. From 220 up to 450 m $\mu$  a hydrogen lamp was used, and for longer wave lengths a tungsten filament was used. The slit width was kept sufficiently small to operate with beams of band width no greater than 1 m $\mu$  at medium intensity. (Fig. 3).

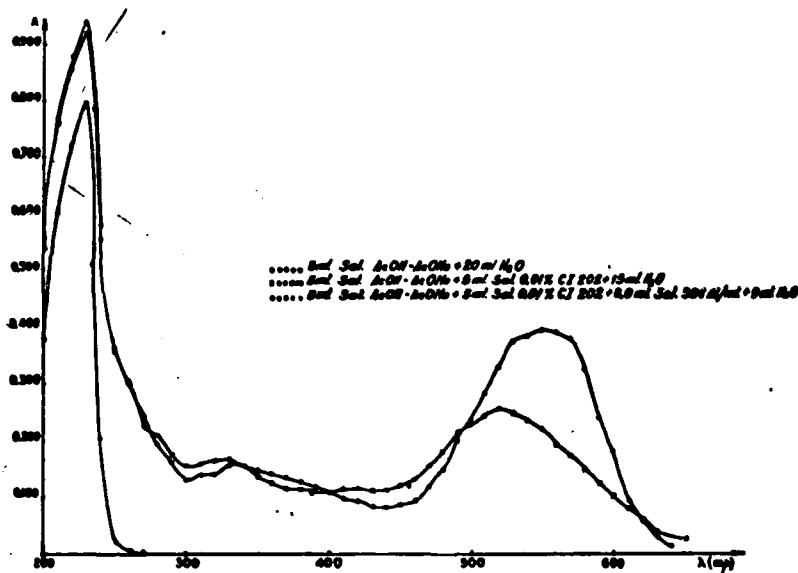


Fig. 3. Absorption spectra.

It can be observed that the peaks of maximum absorption in the visible range occur at 520 m $\mu$  for the coloring agent in deionized water and at 560 m $\mu$  for the complex it forms with aluminum, using the same solvent.

The peak of maximum absorption in samples with excess of coloring agent will depend on the relation complex concentration/coloring agent.

Operating with excess of coloring agent and using a wave length of 560 m $\mu$ , it would be possible to make an absorbchrometric evaluation of aluminum with a sensitivity of the order of 0.01  $\gamma$  of Al/cm<sup>2</sup> [See note]. Both the white and the standard absorb strongly any radiation of wave length smaller than 240 m $\mu$ . (Fig. 4).

[Note:] The possible variation in the sensitivity of the photomultiplier tube at different wave lengths was not considered.

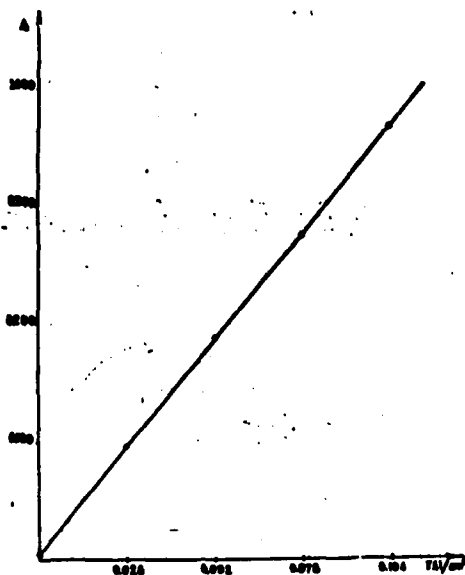


Fig. 4. Curve of absorptometric evaluation of aluminum.

The fluorescence spectra of deionized water, a white solution and a standard solution prepared in the same way were then obtained. In all three cases quartz containers were used, and the samples were irradiated using a mercury lamp No. 2260 with a Corning 9863 filter. This filter permits the passage of radiation of wave length from 230 m $\mu$  to 420 m $\mu$ . (Fig. 5).

From the study of these spectra it can be concluded that the wave length corresponding to maximum (apparent) fluorescence [See note] of the aluminum complex is 605 m $\mu$ . This value depends somehow on the slit width used, since the maximum of  $I_f$  is displaced toward the longer wave length region and the curve becomes relatively flat as the slit width increases. Of course, the displacement of the maximum is due to the fact that the spectrum is not perfectly symmetric with respect to the maximum of  $I_f$ . (Fig. 6).

[Note:] Applying the technique indicated in F. this value may reach 0.005  $\gamma$  Al/cm<sup>2</sup>.

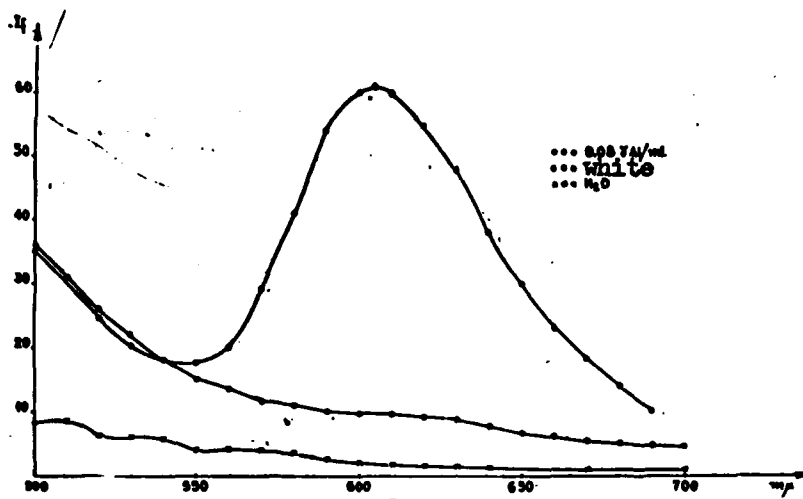


Fig. 5. Fluorescence spectra of deionized water, CI 202 and aluminum complex.

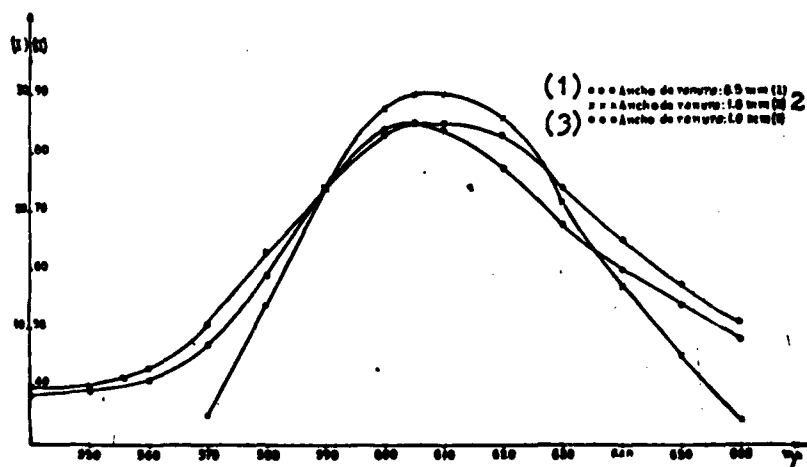


Fig. 6. Influence of slit width on the fluorescence spectrum.

- Legend: 1 - slit width: 0.5 mm (I)  
 2 - slit width: 1.0 mm (II)  
 3 - slit width: 1.0 mm (I)

### E. Study of the Variables of the Analytic Process:

The study and control of the chemical process variables which affect the analytical results is fundamental, and therefore it is our next objective once the optimum wave length for the measurement of fluorescence has been determined. The necessary experiments for the study of every variable were performed keeping the working conditions of the instrument constant, to obtain comparable values.

1) Influence of time in the development of fluorescence. It is well known that the formation of the fluorescent compound is not instantaneous. Therefore, the time required to attain maximum development of fluorescence was determined. The values shown in Table II were obtained by reading fractions of two solutions -- white and standard -- for 48 hours, from the moment volume and homogenization were attained. From this table it can be concluded that to achieve total development at room temperature, about 48 hours are required.

TABLE II

Influence of Time in the Development of Fluorescence

Time	I, White	I, 0.3 $\gamma$ Al/ml
1 minute	2.5	4.5
5 minutes	3.0	7.0
10 "	3.2	8.2
15 "	3.1	12.1
20 "	3.0	14.4
30 "	3.1	17.3
60 "	3.2	23.5
24 hours	4.0	46.2
48 "	5.2	52.3
72 "	5.0	52.0

2) Influence of heating time in a double boiler: White and standard solutions were prepared using 0.4  $\gamma$  Al/ml, and the time of heating in a double boiler was varied. They were cooled in ice water at the end of the heating periods, and the series was read at the end of the experiment. As a result of this, it can be established that a heating time of 10 minutes in a double boiler is enough for the total development of fluorescence.

TABLE III

Influence of the Heating Time

Time (minutes)	I <sub>t</sub> White	I <sub>t</sub> Standard (0.4 γ Al/ml)
1	4.0	45.5
5	4.5	52.5
10	5.0	55.5
15	5.0	55.0
20	4.5	54.0

TABLE IV

Influence of pH

Standard No.	Al γ/ml	pH	I <sub>t</sub>	ΔI <sub>t</sub>
1	0	2.7	10.4	—
2	0.08	2.7	20.0	9.6
3	0	3.8	13.0	—
4	0.08	3.8	41.0	28.0
5	0	4.3	13.0	—
6	0.08	4.3	45.5	32.5
7	0	4.7	13.0	—
8	0.08	4.7	44.5	31.5
9	0	5.0	12.8	—
10	0.08	5.0	44.0	31.2
11	0	5.9	11.0	—
12	0.08	5.9	26.0	15.0

3) Influence of pH: The necessity to operate with a controlled pH is mentioned several times in the bibliography, and 4.5<sup>(2)</sup> or 4.8<sup>(3)</sup> are indicated as maximum values. Experiments were performed and their results are shown in Table IV. White and standard solutions with 0.08 γ Al/ml were prepared in the following way: to a volume of solution convenient for the experiment -- approximately 5 ml -- 5.0 ml of the controlling acetic acetate solution and 5.0 ml. of the 0.01% coloring agent solution were added. To each white and standard solution a convenient volume of approximately 4N sodium hydroxide or hydrochloric acid solution was added to obtain the indicated pH. The volume was changed to 25 ml

with deionized water and the solution obtained was homogenized and heated in a double boiler for 10 minutes. It was then cooled to room temperature using ice water and the  $I_f$ 's of the series were read using a wave length of 605  $\mu$ . From the study of the values of  $\Delta I_f$  at different pH's it seems to be convenient to perform the experiment at pH 4.3. It must be mentioned that when the pH increases, the coloring agent turns to blue-violet and it is destroyed in a completely alkaline medium. This process is accelerated when the solutions are heated.

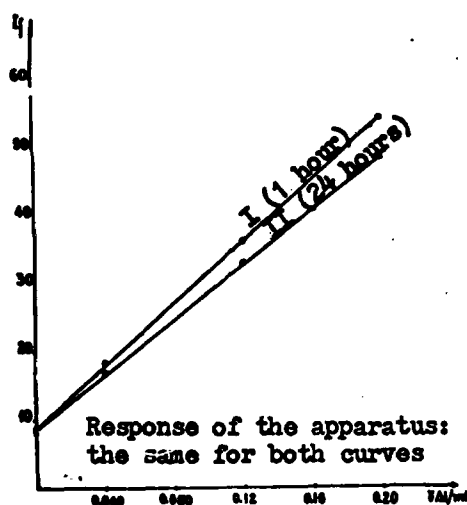


Fig. 7. Stability of fluorescence as a function of time.

4) Fluorescence stability control: A series of readings of several solutions were made, and the values observed in Fig. 7 were obtained. It can be seen that greater differences are produced as the aluminum concentration increases. Anyway, since the proportionality between concentration and fluorescent intensity is maintained, the small instability of  $I_f$  does not prevent the reading of correct values if the standard solutions and the samples are read simultaneously. (Fig. 7).

5) Effects of radiation: A white solution and a standard solution containing 0.04  $\gamma$  of aluminum per ml. were irradiated during longer and longer periods of time. The results obtained show that in the time necessary to take three or four readings of the same solution, no more than a minute, no decrease in  $I_f$  is observed. The effect of a longer exposure time seems to become more important, but the observed decrease in  $I_f$  may be due to an increase in temperature, since the same standard solution heated, but not irradiated, showed smaller values of  $I_f$  ( $\Delta T = 8^\circ\text{C}$ ).



TABLE V

## Influence of the Irradiation Time

Irradiation time	$I_f$	
	White	0.4 $\gamma$ Al/ml.
10 sec.	5.5	42.1
1 min.	5.5	42.0
5 min.	5.6	41.5
10 ..	5.5	41.0

6) Stability of the coloring solution: It was considered convenient to control the influence of time in the CI 202 solution. For this purpose white and standard solutions of the same concentration were prepared, and for every white-standard pair reagent solutions prepared on different days and preserved differently were used. From the values obtained it can be concluded that:

a) the solution gets old, yielding smaller values of  $I_f$  as time goes on.

b) this process is slowed down if the solution is preserved away from light and in a refrigerator.

TABLE VI

## Influence of Time in the Coloring Solution

Series	No.	Age of the CI 202 solution	Preservation	$I_f$		
				White	0.08 $\gamma$ Al/ml	0.4 $\gamma$ Al/ml
1 (*)	1	1 hour	At room temperature, exposed to light	7.5	-	56.0
	2	1 day		7.5	-	55.5
	3	1 month		7.0	-	40.0
	4	2 months		6.0	-	26.5
	5	5 months		5.5	-	14.0
2 (*)	1	1 hour	In refrigerator, shielded from light	10.0	32.0	-
	2	1 day		9.9	32.0	-
	3	1 month		9.8	30.1	-
	4	2 months		9.5	28.0	-

(\*) Series (1) and (2) were obtained separately and with the instrument set for different sensitivity.

7) Influence of the solvent and of the concentration of the CI 202 solution: White and standard solutions of equal concentration were prepared, the CI 202 solutions were prepared as follows:

- i) 0.01% in deionized water.
- ii) 0.1% in deionized water.
- iii) 0.1% in 95° ethyl alcohol.

In the three cases the results obtained were similar. However, the 0.01% aqueous solution was preferred because:

- a) The error in the amount of coloring added is smaller, therefore, the results obtained are less dispersed.
- b) When the standard solutions prepared using the CI 202 alcoholic solution are heated in a double boiler, they boil, which may cause the production of projections.

8) Reproducibility: Repeating the operation five times it was proved that the  $I_T$  produced by white and standard solutions obtained simultaneously are reproducible. The standard deviation expressed in  $\gamma$  Al/ml. is 0.0001 for concentrations of the order of 0.040  $\gamma$  of aluminum per ml. It must be pointed out that in this case the experiment was not performed using the maximum sensitivity of the apparatus.

TABLE VII  
Reproducibility in the Evaluation of Al

Nº	Al ( $\gamma$ /ml.)	$I_T$	Average	e	e <sup>2</sup>	S
1	0	20.0		0	0	
2	0	20.1		+ 0.10	0.01	
3	0	19.9	20.00	- 0.10	0.01	0.07
4	0	20.0		0	0	
5	0	20.0		0	0	
6	0.040	59.1		+ 0.12	0.0144	
7	0.040	59.8	59.98	- 0.18	0.0324	0.13
8	0.040	60.0		+ 0.02	0.0004	
9	0.040	60.1		+ 0.12	0.0144	
10	0.040	59.9		- 0.08	0.0064	

F. Calibration Curves:

Taking into account our conclusions from parts D and E, the details for the procedure to be followed in the evaluation of aluminum with CI 202 were established. Besides, with the instrumental possibilities studied in part C, it was possible to operate in different ranges of concentration of the element under study.

Technique used: To the solution to be evaluated (usually no more than 10 ml.) 5.0 ml. of acetic-acetate controlling solution and 5.0 ml. of 0.01% CI 202 solution in deionized water are added (if it is necessary, the pH is adjusted to 4.3 using a solution of sodium hydroxide or hydrochloric acid with a convenient concentration). The volume is changed to 25 ml. This solution is homogenized and heated in a double boiler for ten minutes. It is then cooled to room temperature in ice water and the  $I_f$  is then read using a wave length of 605 m $\mu$ . White and standard solutions must be handled simultaneously.

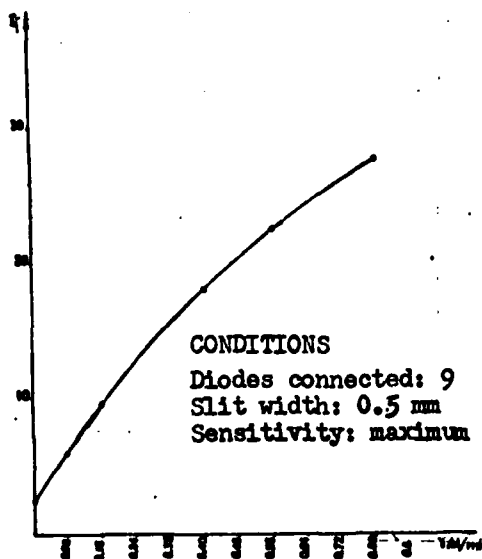


Fig. 8. Calibration curve for concentrations of 0.04-0.08  $\gamma$  of Al/ml.

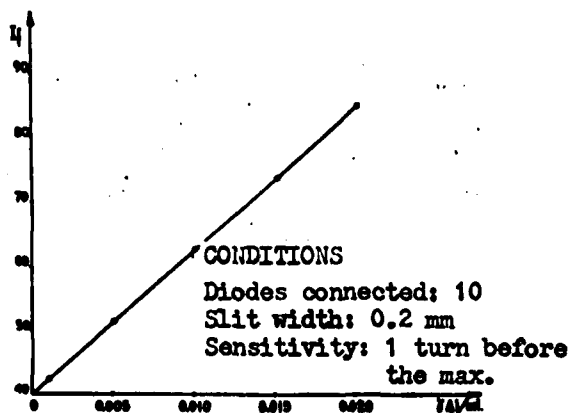


Fig. 9. Calibration curve for low concentrations of aluminum.

The readings obtained using white and standard solutions with increasing concentrations of aluminum may be seen in Figs. 8 [see note] and 9.

[Note:] During the processing of the white and standard solutions corresponding to this curve, 10 ml. of 0.01% CI 202 solution in water were added.

From these figures it can be concluded that:

1) The relation  $I_f$ /aluminum concentration stops being linear when the aluminum concentration is increased. Anyway, it stands to reason that the curve may be used for the evaluation of aluminum, because even when the slope decreases as the concentration of the fluorescent compound increases, the relative error in the determination decreases.

2) The sensitivity obtained under the operating conditions used to obtain the curve shown in Fig. 9 is 0.0001  $\gamma$  of Al/ml.

3) When working in the linear portion of the graph, it will be enough to process a known standard solution together with the sample and interpolate or extrapolate the result.

#### G. Influence of Strange Ions:

The discrepancy observed in the bibliography related to the ions which would interfere in the evaluation of aluminum with CI 202 makes a new study of this problem necessary. The results obtained after studying the influence of several ions are shown in Table VIII. In every case, white and standard solutions with concentration of 0.04  $\gamma$  of aluminum per ml., with and without the ion under study, were processed using the technique described in F.

All the experiments were repeated three times. In some cases slightly and equally increased values are observed in white and standard solutions where the concentration of the interfering ion was increased. If at the same time no variation was observed in the solutions, this could be due to the presence of small quantities of aluminum in the drugs used. It is convenient to remember that any experiment involving the use of acid solutions was done in quartz containers to avoid contamination due to the aluminum present in glass.

From Table VIII it may be concluded that at least up to the concentrations used in the experiments, the following ions do not interfere:  $\text{Li}^+$ ,  $\text{Na}^+$ ,  $\text{K}^+$ ,  $\text{Rb}^+$ ,  $\text{Cs}^+$ ,  $\text{Be}^{++}$ ,  $\text{Mg}^{++}$ ,  $\text{Ca}^{++}$ ,  $\text{Sr}^{++}$ ,  $\text{Ba}^{++}$ ,  $\text{Cd}^{++}$ ,  $\text{BO}_3^{3-}$ ,  $\text{Tl}^+$ ,  $\text{SiO}_3^{2-}$ ,  $\text{Pb}^{++}$ ,  $\text{NO}_3^-$ ,  $\text{PO}_4^{3-}$ ,  $\text{AsO}_4^{3-}$ ,  $\text{SO}_4^{2-}$ ,  $\text{SO}_3^{2-}$ ,  $\text{SeO}_4^{2-}$ ,  $\text{SeO}_3^{2-}$ ,  $\text{Cl}^-$ ,  $\text{Br}^-$ ,  $\text{I}^-$ .

On the other hand,  $\text{Sc}^{3+}$ ,  $\text{Y}^{3+}$ ,  $\text{La}^{3+}$ ,  $\text{Mn}^{++}$ ,  $\text{Ni}^{++}$ ,  $\text{Zn}^{++}$ ,  $\text{Hg}^{++}$ ,  $\text{In}^{3+}$ ,  $\text{Sb}^{3+}$ , and most of the rare earth elements in the table interfere slightly, and their presence can be tolerated when the concentration is small (of the order of 4  $\gamma$  per ml., which would yield aluminum/interference ratios of the order of 1:1000 or even better in some instances, with less than 5% error).

However, the other ions checked interfere considerably, and therefore should not be present. (See Table VIII, page 19 and following.)

TABLE VIII

Element	Ion added	Drugs used	Al/element ratio	Effect on $\gamma$ of Al/ml	Observations
Li	Li+	SO <sub>4</sub> Li <sub>2</sub> ·H <sub>2</sub> O p. a.	0: 1.000 1: 1.000	+ 0.001 + 0.041	Does not interfere
Na	Na+	ClNa p. a.	0: 50.000 1: 50.000	+ 0.001 + 0.041	Idem
K	K+	ClK p. a.	0: 5.000 1: 5.000	0.000 + 0.040	Idem
Rb	Rb+	ClRb p. a.	0: 5.000 1: 5.000	0.000 + 0.040	Idem
Cs	Cs+	ClCs p. a.	0: 5.000 1: 5.000	0.000 + 0.040	Idem
Bc	Bc++	SO <sub>4</sub> Bc·4H <sub>2</sub> O p. a.	0: 1.000 1: 1.000	0.000 + 0.040	Idem
Mg	Mg++	(AcO) <sub>2</sub> Mg·4H <sub>2</sub> O p. a.	0: 5.000 1: 5.000	0.000 + 0.040	Idem
Ca	Ca++	Cl <sub>2</sub> Ca p. a.	0: 5.000 1: 5.000	0.000 + 0.040	Idem
Sr	Sr++	Cl <sub>2</sub> Sr·6H <sub>2</sub> O p. a.	0: 5.000 1: 5.000	0.000 + 0.040	Idem
Ba	Ba++	Cl <sub>2</sub> Ba·2H <sub>2</sub> O p. a.	0: 5.000 1: 5.000	0.000 + 0.040	Idem

TABLE VIII (continued)

Element	Ion added	Drugs used	Al/element ratio	Effect on $I_f$ in $\gamma$ of Al/ml	Observations
Sc	Sc+++	Sc <sub>2</sub> O <sub>3</sub> s.p. ClH p.a. dest.	0: 500 1: 500	+ 0.002 + 0.043	Interferes slightly
Y	Y+++	Cl <sub>3</sub> Y p.a.	0: 1.000 1: 1.000	+ 0.005 + 0.044	Idem
La	La+++	La <sub>2</sub> O <sub>3</sub> s.p. ClH p.a. dest.	0: 1.000 1: 1.000	+ 0.005 + 0.045	Idem
Ti	Ti++++	Ti <sup>+</sup> s.p. SO <sub>2</sub> H <sub>2</sub> p.a. dest.	0: 500 1: 500	— —	Flaky gray-green precipitate
Zr	ZrO++	ZrOCl <sub>2</sub> ·8H <sub>2</sub> O p.a.	0: 500 1: 500	— 0.013 — 0.004	Violet color; stops fluorescence, slight hydrolysis
V	VO <sub>2</sub> <sup>-</sup>	VO <sub>2</sub> Na·4H <sub>2</sub> O p.a.	0: 200 1: 200	— 0.014 — 0.014	Stops fluorescence
Nb	Nb <sup>+</sup>	Cl <sub>5</sub> Nb p.a.	0: 150 1: 150	— 0.003 + 0.014	Turbidness due to hydrolysis, stops fluorescence
Cr	CrO <sub>4</sub> <sup>=</sup>	CrO <sub>4</sub> K <sub>2</sub> p.a.	0: 200 1: 200	— —	Destroys the coloring agent
Mo	Cr+++	(AcO) <sub>3</sub> Cr·H <sub>2</sub> O p.a.	0: 500 1: 500	— 0.004 + 0.027	Blue-violet color, stops fluorescence partially
	MoO <sub>4</sub> <sup>=</sup>	Mo <sub>2</sub> O <sub>7</sub> (NH <sub>4</sub> ) <sub>6</sub> ·4H <sub>2</sub> O p.a.	0: 200 1: 200	— 0.002 + 0.030	Red-violet color, stops fluorescence partially
W	WO <sub>4</sub> <sup>=</sup>	WO <sub>3</sub> I <sub>2</sub> p.a. OHNa p.a. purif.	0: 200 1: 200	— 0.005 + 0.035	Less orange color; stops fluorescence partially

TABLE VIII (continued)

Element	Ion added	Drugs used	Al/element ratio	Effect on $\gamma$ of Al/ml	Observations
Mn	MnO <sub>4</sub> <sup>-</sup>	MnO <sub>4</sub> K p. a.	0: 200 1: 200	—	MnO <sub>2</sub> precipitate destroys the coloring agent
	Mn <sup>++</sup>	SO <sub>4</sub> Mn · 4H <sub>2</sub> O p. a.	0: 200 1: 200 0: 500 1: 500 0: 1,000 1: 1,000	+ 0.001 + 0.041 + 0.004 + 0.046 + 0.009 + 0.053	Lighter color as the Mn <sup>++</sup> concentration increases
Fe	Fe <sup>+++</sup>	(SO <sub>4</sub> ) <sub>2</sub> Fe(NH <sub>4</sub> ) 12H <sub>2</sub> O p. a.	0: 100 1: 100	—	Iron hydrolysis
	Fe <sup>++</sup>	Cl <sub>2</sub> Fe p. a.	0: 500 1: 500	- 0.009 - 0.006	Stops the reaction; brownish color (partially turns to Fe <sup>+++</sup> )
Co	Co <sup>++</sup>	Cl <sub>2</sub> Co · 6H <sub>2</sub> O p. a.	0: 200 1: 200	- 0.013 - 0.013	lavender color. Stops fluorescence
	Ni <sup>++</sup>	Cl <sub>2</sub> Ni · 6H <sub>2</sub> O p. a.	0: 200 1: 200	- 0.001 + 0.038	Does not interfere too much
Ru	Ru <sup>+++</sup>	Cl <sub>2</sub> Ru p. a.	0: 1,000 1: 1,000	- 0.009 + 0.011	More reddish color; stops fluorescence appreciably
	Rh <sup>+++</sup>	Cl <sub>2</sub> Rh p. a.	0: 880 1: 880	- 0.010 - 0.010	Light brown color; stops fluorescence
Rh	Rh <sup>+++</sup>	Cl <sub>2</sub> Rh p. a.	0: 1,000 1: 1,000	- 0.012 - 0.004	More orange color; stops fluorescence

TABLE VIII (continued)

Element	Ion added	Drugs used	Al/element ratio	Effect on $I_f$ in $\gamma$ of Al/ml	Observations
Pt	Pt + + + +	Pt <sup>o</sup> s. p. ClH p. a. dest. NO <sub>3</sub> H p. a. dest.	0: 900 1: 900	-0.027 -0.027	Destroys the coloring agent
Cu	Cu + +	Cl <sub>2</sub> Cu · 2 H <sub>2</sub> O p. a.	0: 200 1: 200	-0.011 -0.011	Stops fluorescence
Ag	Ag +	Ag <sup>o</sup> s. p. NO <sub>3</sub> H p. a. dest.	0: 1.000 1: 1.000	-0.001 +0.026	Destroys the coloring agent (Cl Ag pp. if there are small quantities of Cl <sup>-</sup> in the Cl 202)
Au	Au + + + +	Au <sup>o</sup> s. p. ClH p. a. dest. NO <sub>3</sub> H p. a. dest.	0: 1.000 1: 1.000	-	Destroys the coloring agent forming Au precipitate
Zn	Zn + +	SO <sub>4</sub> Zn · 7 H <sub>2</sub> O p. a.	0: 500 1: 500	+0.003 +0.044	Interferes slightly
			0: 1.000 1: 1.000	+0.009 +0.054	
Cd	Cd + +	CdO p. a. ClH p. a. dest.	0: 1.000 1: 1.000	0.000 +0.040	Does not interfere
Hg	Hg + +	Hg <sup>o</sup> redest. NO <sub>3</sub> H p. a. dest.	0: 500 1: 500	+0.002 +0.043	Makes the solution take a lighter color
			0: 1.000 1: 1.000	-0.002 +0.036	Stops fluorescence partially
B	BO <sub>3</sub> ≡	BO <sub>3</sub> H <sub>3</sub> p. a.	0: 1.000 1: 1.000	+0.001 +0.040	Does not interfere
Ga	Ga + + + +	Ga <sub>2</sub> O <sub>3</sub> s. p. ClH p. a. dest.	0: 20 1: 20	+0.047 +0.079	Interferes because of the fluorescence of the Ga compound with the violet colored Cl 202



TABLE VIII (continued)

Element	Ion added	Drugs used	Al/element ratio	Effect in $I_f$ in $\gamma$ of Al/ml	Observations
In	In +++	In <sub>2</sub> O <sub>3</sub> s. p. ClH p. a. dest.	0: 1.000 1: 1.000	+ 0.007 + 0.047	More violet color. Interferes slightly
Tl	Tl +	NO <sub>3</sub> Tl p. a.	0: 1.000 1: 1.000	0.000 + 0.040	Does not interfere
Si	SiO <sub>3</sub> =	SiO <sub>2</sub> p. a. OHNa p. a. purif.	0: 1.000 1: 1.000	0.000 + 0.040	Idem
Sn	Sn ++	Cl <sub>2</sub> Sn p. a. ClH p. a. dest.	0: 500 1: 500	-- 0.015 -- 0.013	Slight turbidness. Stops fluorescence
Pb	Pb ++	(NO <sub>3</sub> ) <sub>2</sub> Pb p. a.	0: 1.000 1: 1.000	+ 0.003 + 0.043	Less orange color
N	NO <sub>3</sub> -	NO <sub>2</sub> Na p. a.	0: 2.000 1: 2.000	0.000 + 0.040	Does not interfere
	NO <sub>2</sub> -	NO <sub>3</sub> Na p. a.	0: 100 1: 100	-- 0.010 -- 0.010	Destroys the coloring agent
P	PO <sub>4</sub> =	PO <sub>4</sub> H(NH <sub>4</sub> ) <sub>2</sub> p. a.	0: 1.000 1: 1.000	0.000 + 0.040	Does not interfere
As	AsO <sub>4</sub> =	A <sub>3</sub> O <sub>4</sub> HNa <sub>2</sub> · 7H <sub>2</sub> O p. a.	0: 1.000 1: 1.000	0.000 + 0.040	Idem
Sb	Sb +++	Cl <sub>3</sub> Sb p. a. ClH p. a. dest.	0: 500 1: 500	+ 0.002 + 0.044	Interferes slightly
			0: -1.000 1: 1.000	+ 0.006 + 0.047	Interferes slightly

TABLE VIII (continued)

Element	Ion added	Drugs used	Al/element ratio	Effect on $\gamma$ of Al/ml	Observations
Bi	Bi <sup>+++</sup>	Bi <sub>2</sub> O <sub>3</sub> p. a. ClH p. a. dest.	0: 200	-0.002	More violet color; stops fluorescence partially
			1: 200	+0.036	
			0: 500	-0.003	Does not precipitate
			1: 500	+0.030	
S	SO <sub>4</sub> =	SO <sub>4</sub> Na <sub>2</sub> 10 H <sub>2</sub> O p. a.	0: 1.000	0.000	Does not interfere
			1: 1.000	+0.040	
Se	SO <sub>3</sub> =	SO <sub>3</sub> Na <sub>2</sub> p. a.	0: 1.000	-0.001	Idem
			1: 1.000	+0.039	
	SeO <sub>4</sub> =	SeO <sub>4</sub> Na <sub>2</sub> p. a.	0: 1.000	-0.001	Idem
			1: 1.000	+0.039	
	SeO <sub>3</sub> =	SeO <sub>3</sub> Na <sub>2</sub> p. a.	0: 1.000	+0.001	Idem
			1: 1.000	+0.041	
F	F <sup>-</sup>	F(NH <sub>4</sub> ) p. a.	0: 100	-0.018	Stops fluorescence (forming a complex with Al <sup>+++</sup> )
			1: 100	-0.007	
Cl	Cl <sup>-</sup>	ClK p. a.	0: 5.000	0.000	Does not interfere
			1: 5.000	+0.040	
Br	Br <sup>-</sup>	BrNa p. a.	0: 1.000	0.000	Idem
			1: 1.000	+0.041	
I	I <sup>-</sup>	IK p. a.	0: 1.000	0.000	Idem
			1: 1.000	+0.040	
Ce	Ce <sup>+++</sup>	(SO <sub>4</sub> ) <sub>2</sub> Ce p. a. SO <sub>4</sub> H <sub>2</sub> p. a. dest.	0: 500	-0.017	Destroys the coloring agent
			1: 500	-0.017	
	Ce <sup>+++</sup>	(SO <sub>4</sub> ) <sub>2</sub> Ce p. a. SO <sub>3</sub> Na <sub>2</sub> p. a.	0: 200	+0.006	Interferes fairly
			1: 200	+0.046	

Element	Reaction	Flame	Color	Wavelength (nm)	Intensity	Notes
Ba	$\text{BaCl}_2$ s.p.	+	Green	455.4	± 0.01	
	$\text{BaCl}_2$ p.a. dest.	+	Green	455.4	± 0.03	
Ca	$\text{CaCl}_2$ s.p.	+	Red	850.8	± 0.02	
	$\text{CaCl}_2$ p.a. dest.	+	Red	850.8	± 0.03	
Sr	$\text{SrCl}_2$ s.p.	+	Red	467.8	± 0.02	
	$\text{SrCl}_2$ p.a. dest.	+	Red	467.8	± 0.03	
K	$\text{K}_2\text{CO}_3$ s.p.	++	Violet	766.5	± 0.01	
	$\text{K}_2\text{CO}_3$ p.a. dest.	++	Violet	766.5	± 0.04	
Rb	$\text{Rb}_2\text{CO}_3$ s.p.	+++	Violet	780.0	± 0.01	
	$\text{Rb}_2\text{CO}_3$ p.a. dest.	+++	Violet	780.0	± 0.04	
Cs	$\text{Cs}_2\text{CO}_3$ s.p.	+++	Violet	852.1	± 0.01	
	$\text{Cs}_2\text{CO}_3$ p.a. dest.	+++	Violet	852.1	± 0.04	
Li	$\text{LiCl}$ s.p.	++	Red	670.8	± 0.001	
	$\text{LiCl}$ p.a. dest.	++	Red	670.8	± 0.016	
Na	$\text{NaCl}$ s.p.	+++	Yellow	589.0	± 0.003	
	$\text{NaCl}$ p.a. dest.	+++	Yellow	589.0	± 0.043	
Mg	$\text{MgCl}_2$ s.p.	++	Green	448.1	± 0.003	
	$\text{MgCl}_2$ p.a. dest.	++	Green	448.1	± 0.013	
Zn	$\text{ZnCl}_2$ s.p.	++	Blue	481.0	± 0.002	
	$\text{ZnCl}_2$ p.a. dest.	++	Blue	481.0	± 0.013	
Al	$\text{Al}_2\text{O}_3$ s.p.	++	None	508.7	± 0.001	
	$\text{Al}_2\text{O}_3$ p.a. dest.	++	None	508.7	± 0.031	More violet color, stops fluorescence partially
Fe	$\text{FeCl}_3$ s.p.	++	None	447.1	± 0.002	
	$\text{FeCl}_3$ p.a. dest.	++	None	447.1	± 0.027	
Mn	$\text{MnCl}_2$ s.p.	++	None	448.1	± 0.009	
	$\text{MnCl}_2$ p.a. dest.	++	None	448.1	± 0.053	

## CONCLUSIONS

1. The operating conditions of the Beckman spectrophotometer, model DU with attachment for the determination of spectral fluorescence were studied in order to determine its possibilities and limitations. It was concluded that:

a) In most of the cases it is convenient to adjust the sensitivity of the instrument between the midpoint and one turn before reaching the maximum sensitivity of the corresponding potentiometer.

b) It is convenient to connect up to 9 diodes of the photomultiplier tube, leaving the tenth position for cases of extremely low concentrations.

c) It is possible to operate with a slit width between 0.2 and 1.0 mm, according to the aluminum concentration and to the sample composition.

2. The absorption spectra of the reagent and the compound it forms with aluminum in deionized water were obtained. These spectra exhibit maxima at 520 and 560 m $\mu$  respectively. We accept as possible the absorptometric evaluation of aluminum operating against the reagent at a wave length of 560 m $\mu$  (a sensitivity of the order of 0.005  $\gamma$  Al/cm<sup>2</sup> could be obtained using the proposed technique).

3. From the fluorescence spectra of deionized water, a white, and a standard solution, the optimum wave length for the evaluation of the fluorescent complex was established to be 605 m $\mu$ .

4. The variables affecting the values of  $I_f$  obtained were studied, and working techniques were developed.

5. It was shown that the  $I_f$  varies linearly with the aluminum concentration when this one is maintained under 0.2  $\gamma$  of aluminum/ml. For larger concentrations, the calibration curves obtained permit a correct evaluation of aluminum concentration. When operating under adequate conditions it is possible to attain a sensitivity of 0.0001  $\gamma$  Al/ml.

6. The influence of most of the ions potentially present in a sample in highly unfavorable concentrations was controlled, and it was concluded that:

a) Up to concentrations of 40  $\gamma$ /ml the following ions do not interfere: Li<sup>+</sup>, Na<sup>+</sup>, K<sup>+</sup>, Rb<sup>+</sup>, Cs<sup>+</sup>, Be<sup>++</sup>, Mg<sup>++</sup>, Ca<sup>++</sup>, Sr<sup>++</sup>, Ba<sup>++</sup>, Cd<sup>++</sup>, BO<sub>3</sub><sup>3-</sup>, TI<sup>+</sup>, SiO<sub>3</sub><sup>2-</sup>, Pb<sup>++</sup>, NO<sub>3</sub><sup>-</sup>, PO<sub>4</sub><sup>3-</sup>, AsO<sub>4</sub><sup>3-</sup>, SO<sub>4</sub><sup>2-</sup>, SO<sub>3</sub><sup>2-</sup>, SeO<sub>4</sub><sup>2-</sup>, SeO<sub>3</sub><sup>2-</sup>, Cl<sup>-</sup>, Br<sup>-</sup>, I<sup>-</sup>.

b) The following ions interfere slightly, therefore their presence can be tolerated in concentrations up to 4  $\gamma$ /ml:  $\text{Sc}^{3+}$ ,  $\gamma^{3+}$ ,  $\text{La}^{3+}$ ,  $\text{Mn}^{2+}$ ,  $\text{Ni}^{2+}$ ,  $\text{Zn}^{2+}$ ,  $\text{Hg}^{2+}$ ,  $\text{In}^{2+}$ ,  $\text{Sb}^{3+}$ , and most of the rare earth elements which were tried.

c) The following ions interfere seriously and should not be present:  $\text{Ti}^{4+}$ ,  $\text{ZrO}^{++}$ ,  $\text{VO}_3^-$ ,  $\text{Nb}^{5+}$ ,  $\text{CrO}_4^{2-}$ ,  $\text{Cr}^{3+}$ ,  $\text{MoO}_4^{2-}$ ,  $\text{WO}_4^{2-}$ ,  $\text{MnO}_4^-$ ,  $\text{Fe}^{3+}$ ,  $\text{Fe}^{2+}$ ,  $\text{Co}^{++}$ ,  $\text{Ru}^{3+}$ ,  $\text{Rh}^{3+}$ ,  $\text{Pt}^{4+}$ ,  $\text{Cu}^{++}$ ,  $\text{Ag}^+$ ,  $\text{Au}^{3+}$ ,  $\text{Ga}^{3+}$ ,  $\text{Sn}^{++}$ ,  $\text{NO}_2^-$ ,  $\text{Bi}^{3+}$ ,  $\text{F}^-$ ,  $\text{Ce}^{4+}$ ,  $\text{Ce}^{3+}$ ,  $\text{UO}_2^{2+}$ ,  $\text{Th}^{4+}$ .

Acknowledgments. We are grateful to the National Council of Scientific and Technical Investigations for its help, which made possible the acquisition of the necessary equipment, and to the Duperial company, which kindly provided the CI 202 used for the fluorescimetric evaluation of aluminum.

#### BIBLIOGRAPHY

1. White, C. and Lowe, C.: Ind. Eng. Chem., Anal. Ed. 9, 430 (1937).
2. Bourstyn, M.: Mull. Soc. Chim., 8, 540 (1941).
3. Weessler, A. and White, C.: Ind. Eng. Chem., Anal. Ed., 18, 530 (1946).
4. Charlot, G.: Anal. Chim. Acta 1, 218 (1947).
5. Ishibashi, M.; Shigematsu, T. and Nishikawa, Y.: Bunseki Kagaku, 6, 568 (1957).
6. Possidoni de Albinati, Julia Flavia: Anales de la Asociacion Quim. Argentina, 43, 106 (1955).

COLLEGE OF EXACT AND NATURAL SCIENCE  
DEPARTMENT OF INORGANIC, ANALYTIC  
AND PHYSICAL CHEMISTRY

Received: November 1961