

AWARD NUMBER: W81XWH-15-1-0410

TITLE: The Effect of Prosthetic Socket Interface Design on Socket Comfort, Residual Limb Health, and Function for the Transfemoral Amputee

PRINCIPAL INVESTIGATOR: M. Jason Highsmith

CONTRACTING ORGANIZATION: University of South Florida  
Tampa, FL 33612-4766

REPORT DATE: OCTOBER 2019

TYPE OF REPORT: Annual

PREPARED FOR: U.S. Army Medical Research and Materiel Command  
Fort Detrick, Maryland 21702-5012

DISTRIBUTION STATEMENT: Approved for Public Release;  
Distribution Unlimited

The views, opinions and/or findings contained in this report are those of the author(s) and should not be construed as an official Department of the Army position, policy or decision unless so designated by other documentation.

# REPORT DOCUMENTATION PAGE

*Form Approved*  
*OMB No. 0704-0188*

Public reporting burden for this collection of information is estimated to average 1 hour per response, including the time for reviewing instructions, searching existing data sources, gathering and maintaining the data needed, and completing and reviewing this collection of information. Send comments regarding this burden estimate or any other aspect of this collection of information, including suggestions for reducing this burden to Department of Defense, Washington Headquarters Services, Directorate for Information Operations and Reports (0704-0188), 1215 Jefferson Davis Highway, Suite 1204, Arlington, VA 22202-4302. Respondents should be aware that notwithstanding any other provision of law, no person shall be subject to any penalty for failing to comply with a collection of information if it does not display a currently valid OMB control number. **PLEASE DO NOT RETURN YOUR FORM TO THE ABOVE ADDRESS.**

<b>1. REPORT DATE</b> OCTOBER 2019		<b>2. REPORT TYPE</b> Annual		<b>3. DATES COVERED</b> 15-Sep-2018 - 14-Sep-2019	
<b>4. TITLE AND SUBTITLE</b> The Effect of Prosthetic Socket Interface Design on Socket Comfort, Residual Limb Health, and Function for the Transfemoral Amputee				<b>5a. CONTRACT NUMBER</b> W81XWH-15-1-0410	
				<b>5b. GRANT NUMBER</b>	
				<b>5c. PROGRAM ELEMENT NUMBER</b>	
<b>6. AUTHOR(S)</b> Highsmith, M. Jason  E-Mail: mhighsmi@health.usf.edu				<b>5d. PROJECT NUMBER</b>	
				<b>5e. TASK NUMBER</b>	
				<b>5f. WORK UNIT NUMBER</b>	
<b>7. PERFORMING ORGANIZATION NAME(S) AND ADDRESS(ES)</b>  University of South Florida Div Sponsored Research 4202 E. Fowler Avenue Tampa, FL 33620-9951				<b>8. PERFORMING ORGANIZATION REPORT NUMBER</b>	
<b>9. SPONSORING / MONITORING AGENCY NAME(S) AND ADDRESS(ES)</b>  U.S. Army Medical Research and Materiel Command Fort Detrick, Maryland 21702-5012				<b>10. SPONSOR/MONITOR'S ACRONYM(S)</b>	
				<b>11. SPONSOR/MONITOR'S REPORT NUMBER(S)</b>	
<b>12. DISTRIBUTION / AVAILABILITY STATEMENT</b>  Approved for Public Release; Distribution Unlimited					
<b>13. SUPPLEMENTARY NOTES</b>					
<b>14. ABSTRACT</b> Residual limb health and comfort of any person with limb loss of all levels is crucial to achieving maximum prosthetic use and function. There is currently inadequate data substantiating the impact of interface design on socket comfort, residual limb health and function. There are two alternative interface designs for the military and veteran above knee amputee that could provide answers to issues germane to above knee amputees such as moisture control, skin temperature and condition. The Dynamic Socket (DS) design is comprised of a flexible interface and minimal laminated rigid frame to reduce thermal layers, increase flexibility and comfort while retaining ischial containment. In contrast, a Sub-I design has significantly lower trim lines, without ischial containment compared with a traditional interface. However, these alternative designs could compromise overall function compared to the standard of care interface design. Therefore the focus of this clinical trial is to determine if the DS and Sub-I alternative interface designs will improve socket comfort, residual limb health and function compared to the standard of care IRC interface design.					
<b>15. SUBJECT TERMS: NONE LISTED</b>					
<b>16. SECURITY CLASSIFICATION OF:</b>			<b>17. LIMITATION OF ABSTRACT</b>	<b>18. NUMBER OF PAGES</b>	<b>19a. NAME OF RESPONSIBLE PERSON</b>
<b>a. REPORT</b>	<b>b. ABSTRACT</b>	<b>c. THIS PAGE</b>			USAMRMC
Unclassified	Unclassified	Unclassified	Unclassified	7	<b>19b. TELEPHONE NUMBER</b> (include area code)

## Table of Contents

	<b>Page</b>
<b>1. Introduction .....</b>	<b>2</b>
<b>2. Keywords .....</b>	<b>2</b>
<b>3. Accomplishments .....</b>	<b>2</b>
<b>4. Impact.....</b>	<b>3</b>
<b>5. Changes/Problems.....</b>	<b>3</b>
<b>6. Products.....</b>	<b>4</b>
<b>7. Participants &amp; Other Collaborating Organizations .....</b>	<b>4</b>
<b>8. Special Reporting Requirements.....</b>	<b>6</b>
<b>9. Appendices .....</b>	<b>6</b>

## 1. INTRODUCTION:

Residual limb health and comfort of any person with limb loss of all levels is crucial to achieving maximum prosthetic use and function. There is currently inadequate data substantiating the impact of interface design on socket comfort, residual limb health and function. There are two alternative interface designs for the military and veteran above knee amputee that could provide answers to issues germane to above knee amputees such as moisture control, skin temperature and condition. The Dynamic Socket (DS) design is comprised of a flexible interface and minimal laminated rigid frame to reduce thermal layers, increase flexibility and comfort while retaining ischial containment. In contrast, a Sub-I design has significantly lower trim lines, without ischial containment compared with a traditional interface. However, these alternative designs could compromise overall function compared to the standard of care interface design. Therefore the focus of this clinical trial is to determine if the DS and Sub-I alternative interface designs will improve socket comfort, residual limb health and function compared to the standard of care IRC interface design.

## 2. KEYWORDS: Provide a brief list of keywords (limit to 20 words).

prosthetic socket, interface, perspiration, residual limb, comfort, health, vacuum-assisted suspension, brimless

## 3. ACCOMPLISHMENTS:

### What were the major goals of the project?

**Primary Aim:** To determine if military and veteran transfemoral amputees of non-dysvascular etiology will experience improved residual limb health following accommodation with DS and Sub-I interfaces compared to the standard of care IRC interface. In order to address the primary aim, research question (RQ) #1 was posed:

RQ #1. Compared to the standard of care IRC interface, do DS and Sub-I interfaces decrease:

- a. skin temperature?
- b. perspiration?
- c. vertical interface movement (pistoning)?

**Secondary Aim #1:** To determine if military and veteran transfemoral amputees of non-dysvascular etiology will demonstrate increased function following accommodation with DS and Sub-I interfaces compared to the standard of care IRC interface. In order to address Secondary Aim #1, RQ #2 was posed:

RQ #2. Compared to the standard of care IRC interface, do DS and Sub-I interfaces improve:

- a. balance and stability?
- b. mobility?

**Secondary Aim #2:** To determine if military and veteran transfemoral amputees of non-dysvascular etiology will prefer DS or Sub-I interfaces compared to the standard of care IRC interface, following accommodation. In order to address Secondary Aim #2, RQ #3 was posed:

RQ #3. In the short and long term, compared to the standard of care IRC interface, are DS and Sub-I

interfaces:

- a. more comfortable?
- b. preferred?

### **What was accomplished under these goals?**

Both aims above have been completed at this time with most data analysis complete and two (2) publications submitted. Findings included that medial socket wall height was significantly different between the 3 experimental sockets ( $p < .05$ ). There were no differences in femoral adduction angle, ischial containment or other imaging findings between interventions. Preliminary analysis of balance/Neurocom data reveal that amputees had more falls while using the brimless socket. Statistical analyses ongoing.

Study tasks 1, 2a, 2b, and 2c as presented in the Statement of Work are complete. Task 3b (dissemination) is ongoing, as one more publication will be submitted shortly. Task 3d, translating plans back to stakeholders, is ongoing. DOD representatives (Jason Ghannadian) approved use of study funds to host a consensus conference focusing on transfemoral socket designs and considerations. The consensus conference was held August 26 and 27, 2019. Author team manuscripts and the final manuscript by the study co-chairs will be completed and submitted in November 2019.

### **What opportunities for training and professional development has the project provided?**

A Mechanical Engineering undergraduate student was hired to assist with lab setup, equipment calibration, data collection, and data management and analysis. As part of these duties, the student learned to interact with human subjects as well as how to manage data and prepare it for analysis. He continues to be instrumental in the preparation, analysis, and dissemination of the study data. Additionally, the study PI, co-PI, and research coordinator attended the American Academy of Orthotists & Prosthetists (AAOP) annual meeting, March 6-9, 2019, Orlando, FL. The study team disseminated study results took part in professional development by attending sessions discussing latest scientific developments regarding transfemoral prosthetics.

### **How were the results disseminated to communities of interest?**

The PI and co-PI presented study results at AOPA National Assembly, September 26-29, 2018, Vancouver, British Columbia, Canada and at the American Academy of Orthotists & Prosthetists (AAOP) annual meeting, March 6-9, 2019, Orlando, FL.

### **What do you plan to do during the next reporting period to accomplish the goals?**

At this point, final data analysis and knowledge dissemination continue. Currently, we are analyzing dermatology, perspiration, and subjective (surveys) portions of the data.

## **4. IMPACT:**

### **What was the impact on the development of the principal discipline(s) of the project?**

Nothing to report at this time.

### **What was the impact on other disciplines?**

Nothing to report at this time.

### **What was the impact on technology transfer?**

Nothing to report at this time.

### **What was the impact on society beyond science and technology?**

Nothing to report at this time.

## **5. CHANGES/PROBLEMS:**

### **Changes in approach and reasons for change**

Nothing to report at this time.

### **Actual or anticipated problems or delays and actions or plans to resolve them**

Nothing to report at this time

### **Changes that had a significant impact on expenditures**

Nothing to Report

### **Significant changes in use or care of human subjects, vertebrate animals, biohazards, and/or select agents**

Nothing to Report

## **6. PRODUCTS:**

### **• Publications, conference papers, and presentations**

Highsmith MJ(chair/moderator), Klenow TD, Kahle JT, Wernke M. Prosthetic Socket Design Impact on the Amputee User in the Laboratory and Clinic. Symposium (C15). Sept 2018. American Orthotics & Prosthetics Association (AOPA) National Assembly. Vancouver, B.C. Canada

Kahle JT, Miro RM, Ho LT, Porter M, Lura DJ, Carey SL, Lunseth P, Swanson A, Highsmith MJ. The effect of above the knee prosthetic socket interface design on gait, balance, mobility, and preference: randomized clinical trial. Pros Orth Int, Submitted, July 2019

Publications in process include: (1) Physical functional performance measures, and (2) Temperature responses.

### **Books or other non-periodical, one-time publications.**

Nothing to report at this time.

### **Other publications, conference papers, and presentations.**

Publications resulting from the Multi-Sector State of the Science Conference: Transfemoral Socket Design and Considerations will include the following topics (full titles to be determined):

- Critical Design Features/Socket Variations
- Heat Retention/Perspiration/Dermatologic Concerns
- Surgical Variations and Prescription Recommendations
- Suspension/Interface Issues
- Alignment, Movement Constraints, and Compensatory Strategies
- Considerations for the Female using a Transfemoral Prosthesis
- Clinical, Regulatory, Ethical and Other Considerations with Osseointegration

- **Website(s) or other Internet site(s)**

Nothing to report.

- **Technologies or techniques**

Nothing to report.

- **Inventions, patent applications, and/or licenses**

Nothing to report.

- **Other Products**

Nothing to report.

## **7. PARTICIPANTS & OTHER COLLABORATING ORGANIZATIONS**

### **What individuals have worked on the project?**

Name: Jason Highsmith

Project Role: Principal Investigator

Researcher Identifier: N/A

Nearest person month worked: 1 calendar month

Contribution to Project: Coordinated and planned project with the members of the research team. Submitted institutional and DOD IRBs and ClinicalTrials.gov registry. Tested study thermistor with Dr. Lura (see below). Data analysis and knowledge dissemination (publication and presentations).

Name: Rebecca Miro

Project Role: Research Coordinator

Researcher Identifier: N/A

Nearest person month worked: 1 calendar month

Contribution to Project: Managed set-up and execution of 4 study subcontracts. Worked with Dr. Highsmith to submit IRB applications and ClinicalTrials.gov registry. Assisted Dr. Highsmith with data collection.

Name: Derek Lura

Project Role: Subcontract PI (Florida Gulf Coast University)

Researcher Identifier: N/A

Nearest person month worked: 0.5 calendar month

Contribution to Project: Designed, built, and tested the thermistor that will be used to record temperature during treadmill walking.

Name: Loi Ho

Project Role: Study Prosthetist

Researcher Identifier: N/A

Nearest person month worked: 2 person months

Contribution to Project: As the study prosthetist, Ms. Ho measured, cast, fabricated and fit sockets for enrolled subjects.

Name: Stephanie Carey

Project Role: Collaborator, Mechanical Engineering

Researcher Identifier: N/A

Nearest person months worked: 0.6 cal months

Contribution to project: Collaboration with research team regarding preliminary data analysis. Mentoring undergraduate student.

Name: Michael Porter

Project Role: Undergraduate student, Mechanical Engineering

Research Identifier: N/A

Nearest person months worked: 0.6 calendar months

Contribution to project: De-identifying and processing data from various outcome measures.

Preparing all study data for processing and preliminary data analysis. Literature searches.

**Has there been a change in the active other support of the PD/PI(s) or senior/key personnel since the last reporting period?**

No.

**What other organizations were involved as partners?**

Organization Name: Florida Gulf Coast University

Location: Fort Myers, FL

Financial Support: None

In-Kind Support: None

Facilities: None

Collaboration: None

Personnel Exchanges: None

Organization Name: Prosthetic Design & Research

Location: Tampa, FL

Financial Support: None

In-Kind Support: None

Facilities: None

Collaboration: None

Personnel Exchanges: None

Organization Name: Tampa VA Research & Education Foundation

Location: Tampa, FL

Financial Support: None

In-Kind Support: None

Facilities: None

Collaboration: None

Personnel Exchanges: None

**8. SPECIAL REPORTING REQUIREMENTS: None**

**9. APPENDICES:** Attach all appendices that contain information that supplements, clarifies or supports the text. Examples include original copies of journal articles, reprints of manuscripts and abstracts, a curriculum vitae, patent applications, study questionnaires, and



# The effect of prosthetic socket interface design on socket comfort, residual limb health, and function for the transfemoral amputee

Log No. MR140125; Award Number: W81XWH-15-1-0410



PI: M. Jason Highsmith, PhD, DPT, CP, FAAOP

Org: University of South Florida


Award Amount: \$912,628

## Study/Product Aim(s)

1. To determine if TFAs will demonstrate decreased RL skin temperature and perspiration following accommodation with a brimless VAS and flexible interface/ rigid frame design with windows interface compared to the current standard of care IRC. 2. To determine if TFAs will demonstrate increased *stability, mobility, gait, comfort, function and quality of life* following accommodation with a brimless VAS and flexible interface/ rigid frame design with windows interface compared to the current standard of care IRC.

## Approach

Active, separated and retired military TFAs will be recruited for this study. The study will involve 15 TFA human subjects. Three different interface designs will be tested: IRC suction sockets, IRC sockets with roll on silicone suspension and windows created in the frame, and VAS brimless. Subjects will serve as their own controls in this A-B-C crossover clinical trial. Subjects will be randomized regarding the crossover sequence through the 3 interface designs.

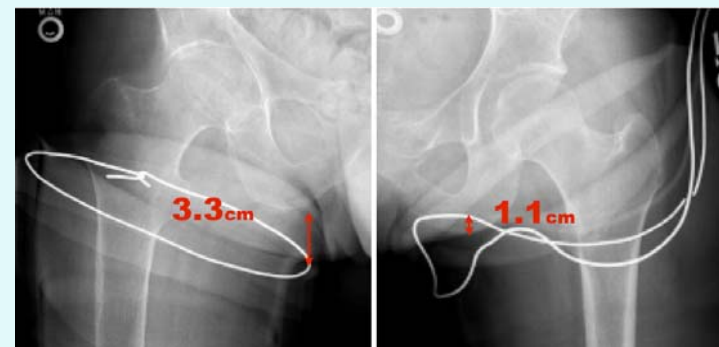

(Left) Windows created in a TFA interface design (Middle), Brimless VAS, vs. (Right) IRC, relative to the IT, the brimless interfaces were an average of 4.4 cm lower than IRC.

## Timeline and Cost

Activities	CY	15	16	17	
Obtain regulatory approvals, begin recruitment		■			
Ongoing recruitment & data collection. Begin data analysis			■		
Complete data collection & analysis. Dissemination				■	
<b>Estimated Budget (\$912.6K)</b>		<b>\$100</b>	<b>\$500</b>	<b>\$300</b>	

Updated: Tampa, FL 09/09/2019

## Goals/Milestones (Example)

**CY15 Goals** – Complete regulatory approvals, begin recruitment

**CY16 Goal** – Continue recruitment, data collection, and begin data analysis.

**CY17 Goal** – Complete data collection and data analysis. Disseminate study findings.

## Comments/Challenges/Issues/Concerns

- Due to the delayed start as the result of regulatory approvals, a no cost extension may be needed.

## Budget Expenditure to Date

Expenditures to date: \$752,901.68