

AD-A045 155

ARMY MEDICAL INTELLIGENCE AND INFORMATION AGENCY WAS--ETC F/G 13/11
VACUUM PUMP MADE OF METAL (VAKUUM PUMPE AUS METALL), (U)
AUG 77 SCHELL

UNCLASSIFIED


USAMIIA-K-8358-B

NL

1 of 1
AD
A045 155



END
DATE
FILMED
11 - 77
DDC

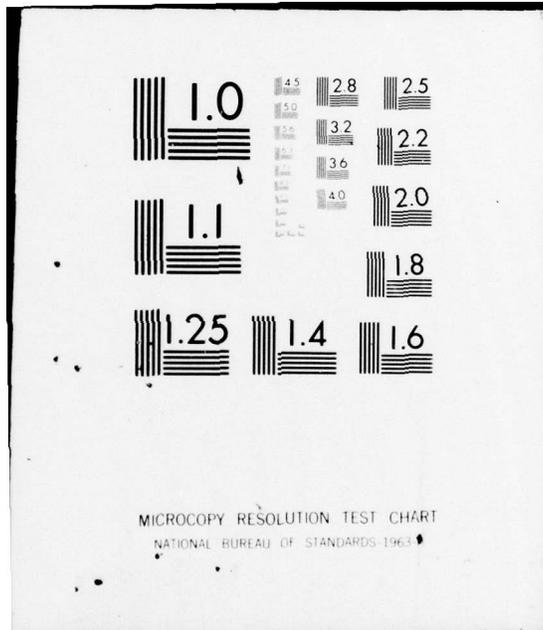

MICROCOPY RESOLUTION TEST CHART
NATIONAL BUREAU OF STANDARDS-1963-A



DEPARTMENT OF THE ARMY
U.S. ARMY MEDICAL INTELLIGENCE AND INFORMATION AGENCY
WASHINGTON, D.C. 20314

1

AD A 045155

Number: 14 USAMIIA TRANSLATION
USAMIIA-K-8358-B

Date Completed: 11 31 Aug 1977

Language: German

12 4 p.

Geographic Area:

English Title: 6 VACUUM PUMP MADE OF METAL
(Vakuumpumpe aus Metall)

Author: 10 LTC Schell

Source Document:

Pages Translated: All (3)

Publisher: 21 Trans. of report from
Academy for Medical Service and Sanitation
of the Bundeswehr (West Germany) Sp.
Date/Place Publication: 28 June 1976, Munich

Distribution Statement: Approved for public release;
distribution unlimited

DDC
OCT 14 1977
A

DDC FILE COPY



409112



Study Group for Medical Technology
and Medical Supplies
(SanTechnik SanMaterial)
Department for Studies and Science
Academy for Medical Service and Sanita-
tion of the Bundeswehr (SanAkBw)
Ref.: 90-65-15

8 Munich 40, 28 June 1976 /1

Infanteriestrasse 17
P.O.B. 400035
Telephone: 089/3870/2625
De/br

To:


Federal Office for Military Technology and Procurement
(Bundesamt fuer Wehrtechnik und Beschaffung) (2 copies)
- BA IV 2 -
Am Rhein 2-4, 5400 Coblenz

Subject: Vacuum Pump Made of Metal

References: 1. BWB - BA IV 2 - Ref. No. 90-65-15 of 21 June 1976
2. Academy for Medical Service and Sanitation of the
Bundeswehr/Department for Studies and Science (ASW),
Study Group for Medical Technology and Medical Sup-
plies, Ref. No. 90-65-15-25 of 24 March 1976

Enclosure: 1. Technical Drawing

Reference 1 requests the Academy for Medical Service and Sanitation
of the Bundeswehr through the Federal Office for Military Technology and
Procurement (BWB) to test a vacuum pump made of metal (as in reference 2)
to establish whether the model fulfills the requirements.

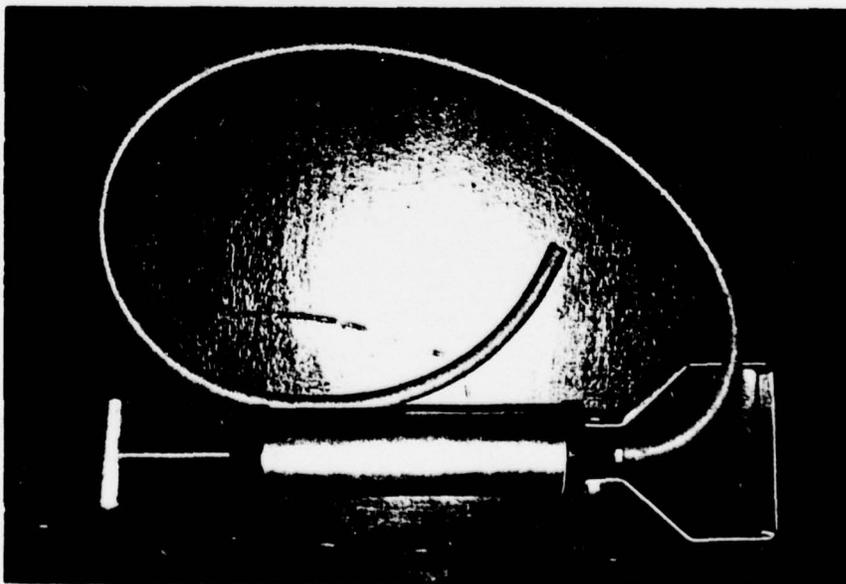

The following position has been established on this matter:

/2

The model demonstrated is stable, has a good suction performance and is basically suited for manual and treadle operation.

However, in order for the pump to be still better utilized for manual and treadle operation and to enable a simple harmless attachment to the vacuum stretcher, the following changes are proposed: (cf. technical drawing as inclosure on this subject*)

1. The foot section should be kept narrower in the width of the area for the foot and be provided with a nonskid rubber or plastic inlay.
2. The web edges should be flanged for increasing web stability.
3. The width of the treadle should remain on the body of the pump as in the model in order for the treadle to keep enough buckling strength.

A pressure hose used as general supply article in the Bundeswehr should be utilized as pump hose.

For

[Signature]

(Schell)


Lieutenant Colonel (Pharmacist)

[Handwritten note: Handpump shipped by separate mail.]

*Translator's Note: Handwritten note.

Inclosure to ltr Anlage zu Schreiben
 Dept for Studies and Science/Academy StudGrp SanTSanMat
 for Med. Service and Sanitation of ASW/SanAKBw
 the Bundeswehr

Az.: 90-65-15 vom 28.06.76
 Ref. No. ... of

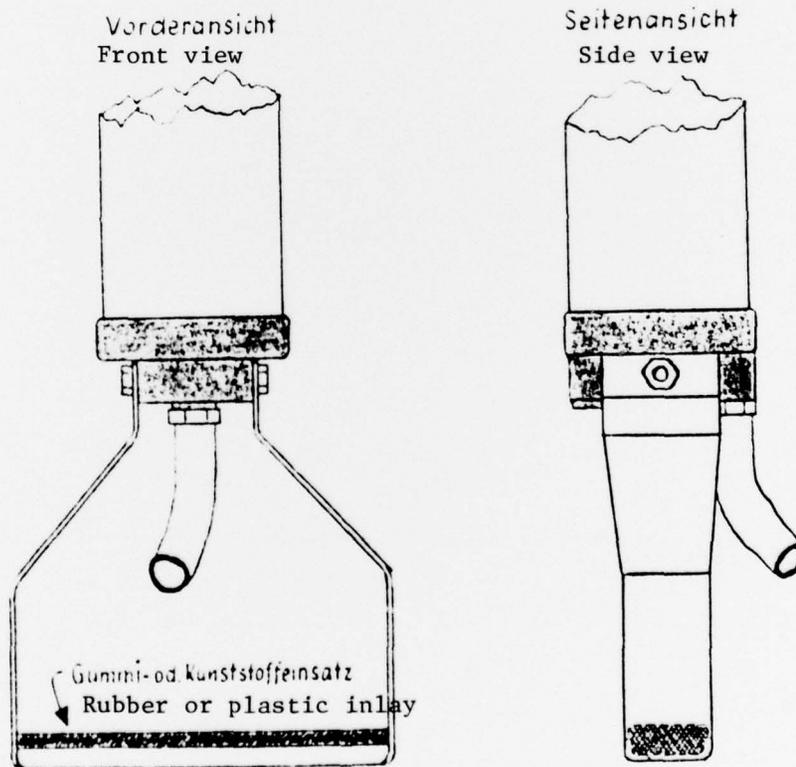

Proposed modification:
 Treadle vacuum pump,
 metal

Änderungsvorschlag:

Fußbügel
 Vakuumpumpe, Metall

Scale: M 1:2,5

1:2.5 SanAKBw ASW
 Studiergruppe
 Sanitätstechnik u Sanitätsmaterial