

AD-A128 862

ADJUSTABLE CARDBOARD DENTAL CHAIR AND STOOL(U) NAVAL  
DENTAL RESEARCH INST GREAT LAKES IL R 5 BAYCAR ET AL.  
FEB 83 NDRI-PR-83-84


1/1

UNCLASSIFIED

F/G 6/5

NL



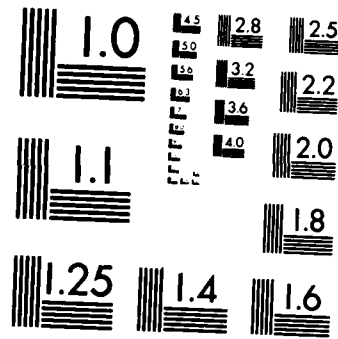

MICROCOPY RESOLUTION TEST CHART  
NATIONAL BUREAU OF STANDARDS-1963-A

20

NDRI-PR 83-04  
FEBRUARY 1983



# ADJUSTABLE CARDBOARD DENTAL CHAIR AND STOOL

DTIC FILE COPY DA 128862

R. S. BAYCAR  
F. AKER  
A. SEROWSKI  
G. BAILEY

DTIC  
COLLECTED  
JUN 3 1983

A

NAVAL  
DENTAL RESEARCH  
INSTITUTE

Naval Medical Research and Development Command  
Bethesda, Maryland

83 00 1 048

NAVAL DENTAL RESEARCH INSTITUTE  
NAVAL BASE, BUILDING 1-H  
GREAT LAKES, ILLINOIS 60088

ADJUSTABLE CARDBOARD DENTAL CHAIR AND STOOL


R. S. BAYCAR  
F. AKER  
A. SEROWSKI  
G. BAILEY

Research Progress Report NDRI-PR 83-04  
Work Unit M093PN002.0001  
Naval Medical Research and Development Command  
National Naval Medical Center  
Bethesda, Maryland 20814

The opinions expressed herein are those of the authors and cannot be construed as reflecting the views of the Navy Department or the Naval Service at large. The use of commercially available products does not imply endorsement of these products or preference to other similar products on the market.

This document has been approved for public release; its distribution is unlimited.

Approved and released by:



G. E. CLARK  
Captain, Dental Corps,  
United States Navy  
Commanding Officer

Portability of dental equipment is a priority for those who provide care to the home-bound, nursing homes, hospitals, rural areas and deployed military. A portable dental chair should be easily transportable, suited for its purpose and be cost effective.

A simple lightweight, adjustable, compact chair constructed from corrugated cardboard has been designed at the Naval Dental Research Institute, Great Lakes, Illinois. The double-ply corrugated cardboard sheets are commercially available and the component parts may be cut out with a sharp knife (1). The chair is designated as the mobile oral treatment and examination chair (MOTEC).

#### Component Parts

The MOTEC is designed to support an adult patient with a maximum weight of 300 pounds. It is adjustable from a reclining to an upright position, which is a feature not included in a previous design (2).

A cardboard stool for the dentist is incorporated in the design to provide a seat when treating a reclining patient. For the seated dentist, this new design allows leg room under the patient's head. When the stool is disassembled, its three component parts are utilized as supports for the chair back when placed in the upright position.

Two 7'x10' sheets of double wall corrugated fiber board (cardboard) with a test strength of 500 pounds per square inch are required for fabrication. Eight cardboard parts are prepared for the construction of one patient chair. Five patterns, (Figures 1-5), are used as guides in making these parts. To prevent excessive waste of material, the pattern drawings are strategically layed out on one sheet of cardboard. For sturdy construction, the corrugations must run in the direction indicated by arrows in the pattern diagrams.

Make one of each of the following: (Figure 1) seat-leg rest; (Figure 2) backrest. Make two of each: (Figure 3) vertical leg support; (Figure 4) vertical back support; (Figure 5) cross support. Three different parts are used to construct the stool. Make one of each: (Figures 6-8). Two of these can be laid out on the unused portion of the first 7'x10' sheet, and the third section on the unused portion of a sheet used to make a second chair. The component parts are cut from the cardboard sheet with a sharp utility knife and stored in a cardboard carrying case.

Moisture deterioration of cardboard in damp environments can be a problem, particularly at the cut edges of each part. For these climatic conditions, we suggest the use of masking tape and a water resistant sealant spray around the exposed edges, especially on the lower portions of the chair and stool.

#### Assembly

Because of design simplicity, the chair can be assembled by one person in less than five minutes. Using the assembly diagram as a guide (Figure 9), begin with the two vertical back supports which are bent at the dotted lines as indicated in the pattern. Note that the folds on one vertical

back support are bent away from you and the folds on the second are bent toward you, forming mirror image parts. After placing them side by side, the cross support is inserted into the slots to secure this segment of the chair base.

Similarly, the vertical leg supports are secured with a cross support to form the second segment of the chair base.

The two base segments are then placed together with the slots on the adjoining free ends aligned. After folding at the locations indicated, the backrest and the seat-leg rest are inserted into the base slots, securing the chair in the reclining position.

The stool used for sit-down dentistry, when the patient is in the reclining position, is fabricated from three parts (Figure 10). Individually, these parts form a brace which holds the back support in the upright position when the stool is not needed (Figure 10).

The total weight of the chair and stool in the carrying case is 20 pounds. When disassembled, the parts occupy a space 40"L x 26"H x 6"W. As we have found from experience, transportation of this equipment can be handled by one person and the total package, including the carrying case, will fit into a small car.

#### Summary

A lightweight cardboard chair has been developed for use in portable dental care delivery programs. The design will accommodate an adult patient, is sturdy, and includes a reclining and an upright position. A stool has been added to the design for sit-down dentistry, and when disassembled, the stool component parts are used as supports for the upright backrest.

#### Acknowledgement

The authors are grateful for the assistance of DT3 Timothy Barnes for the drafting of construction plans; HM1 Eric Larson for photographic support; and Myra Rouse for manuscript preparation.

#### References

1. Hennessey, J. and Papanek, V. Nomadic Furniture. New York, Pantheon Books, 1972.
2. Goldstein, C. M. Design of a practical dental chair made of corrugated cardboard. JADA 97(6):996, December 1978.



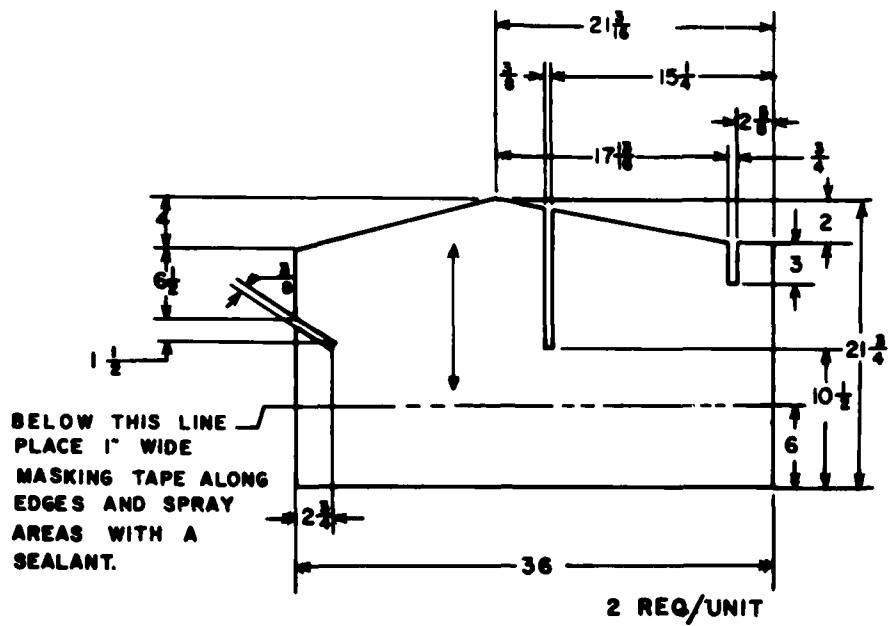


Figure 3. Vertical leg support.

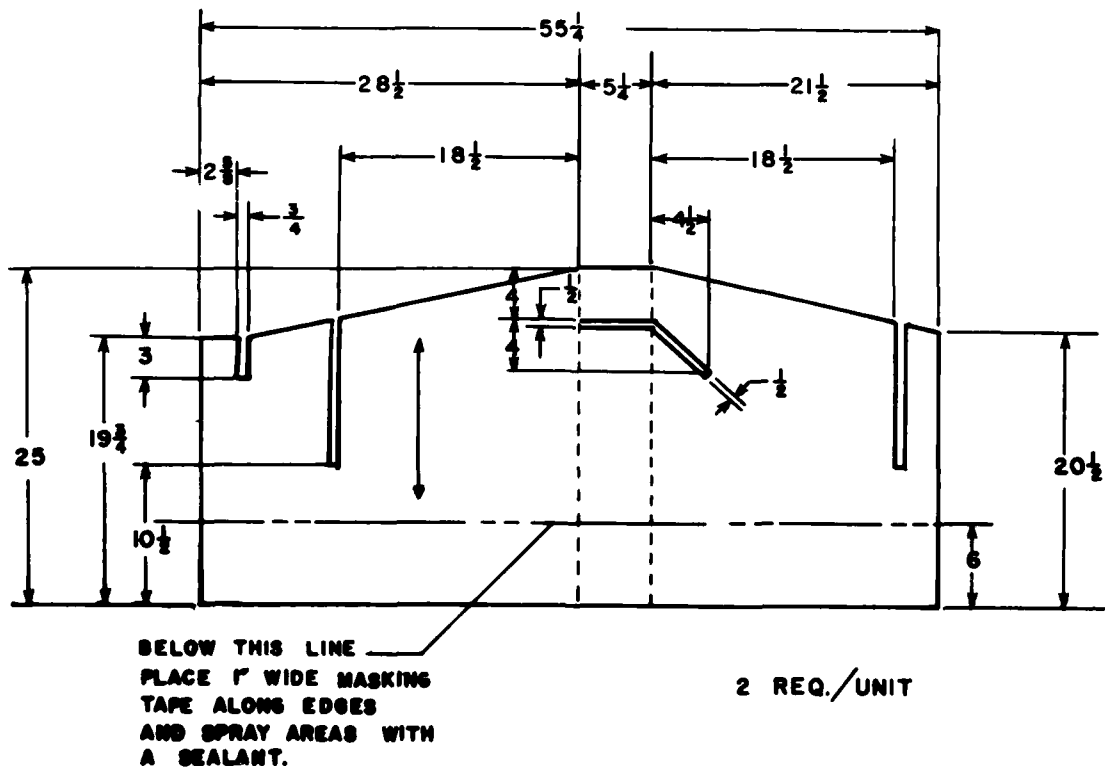


Figure 4. Vertical back support.





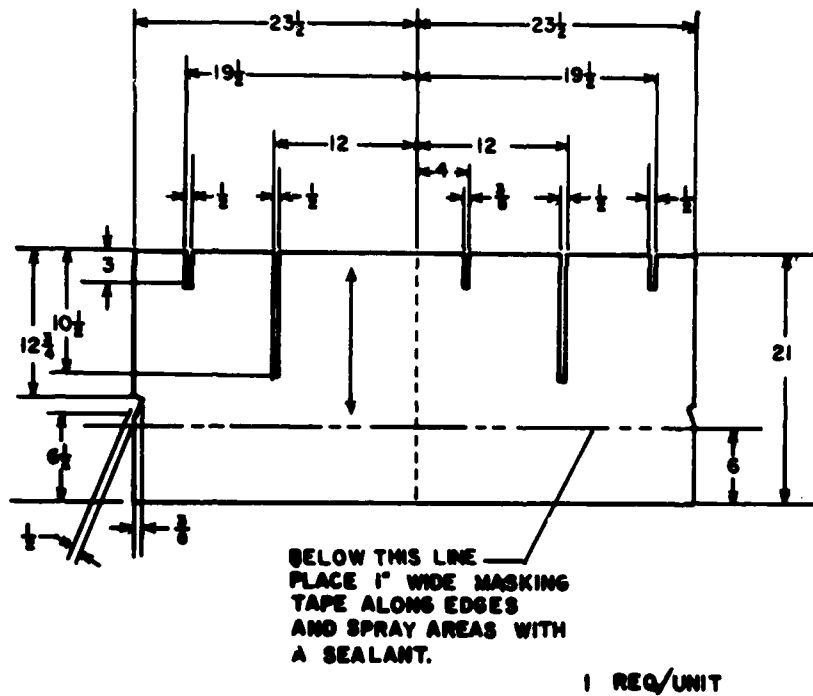


Figure 7. Vertical stool support.

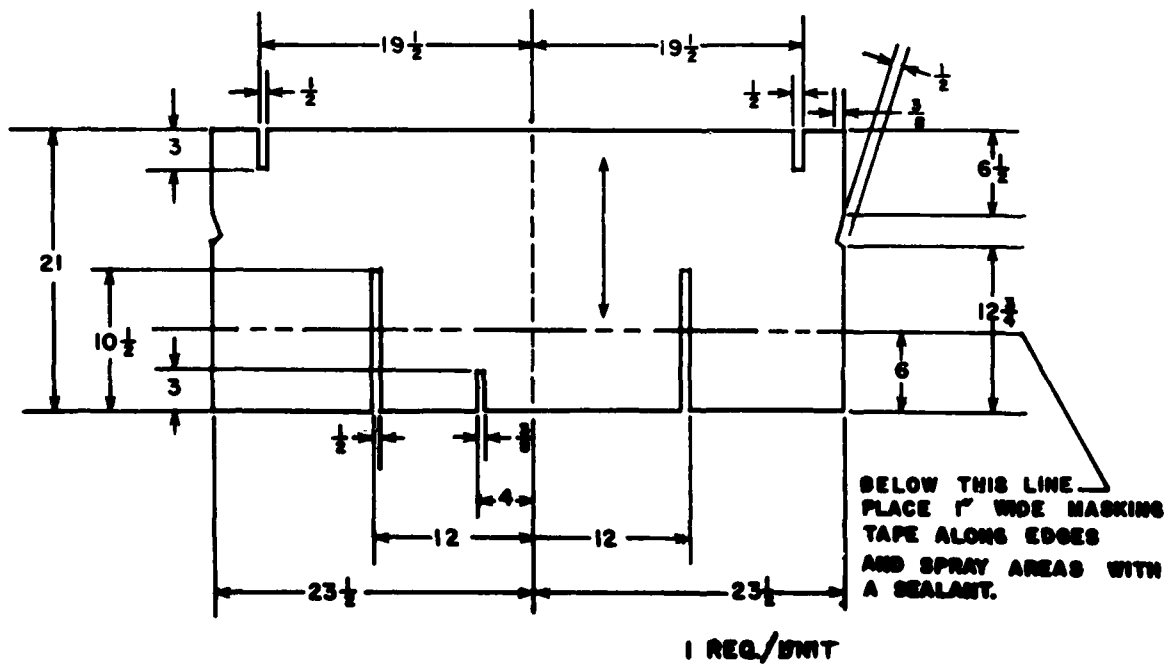


Figure 8. Vertical stool support.

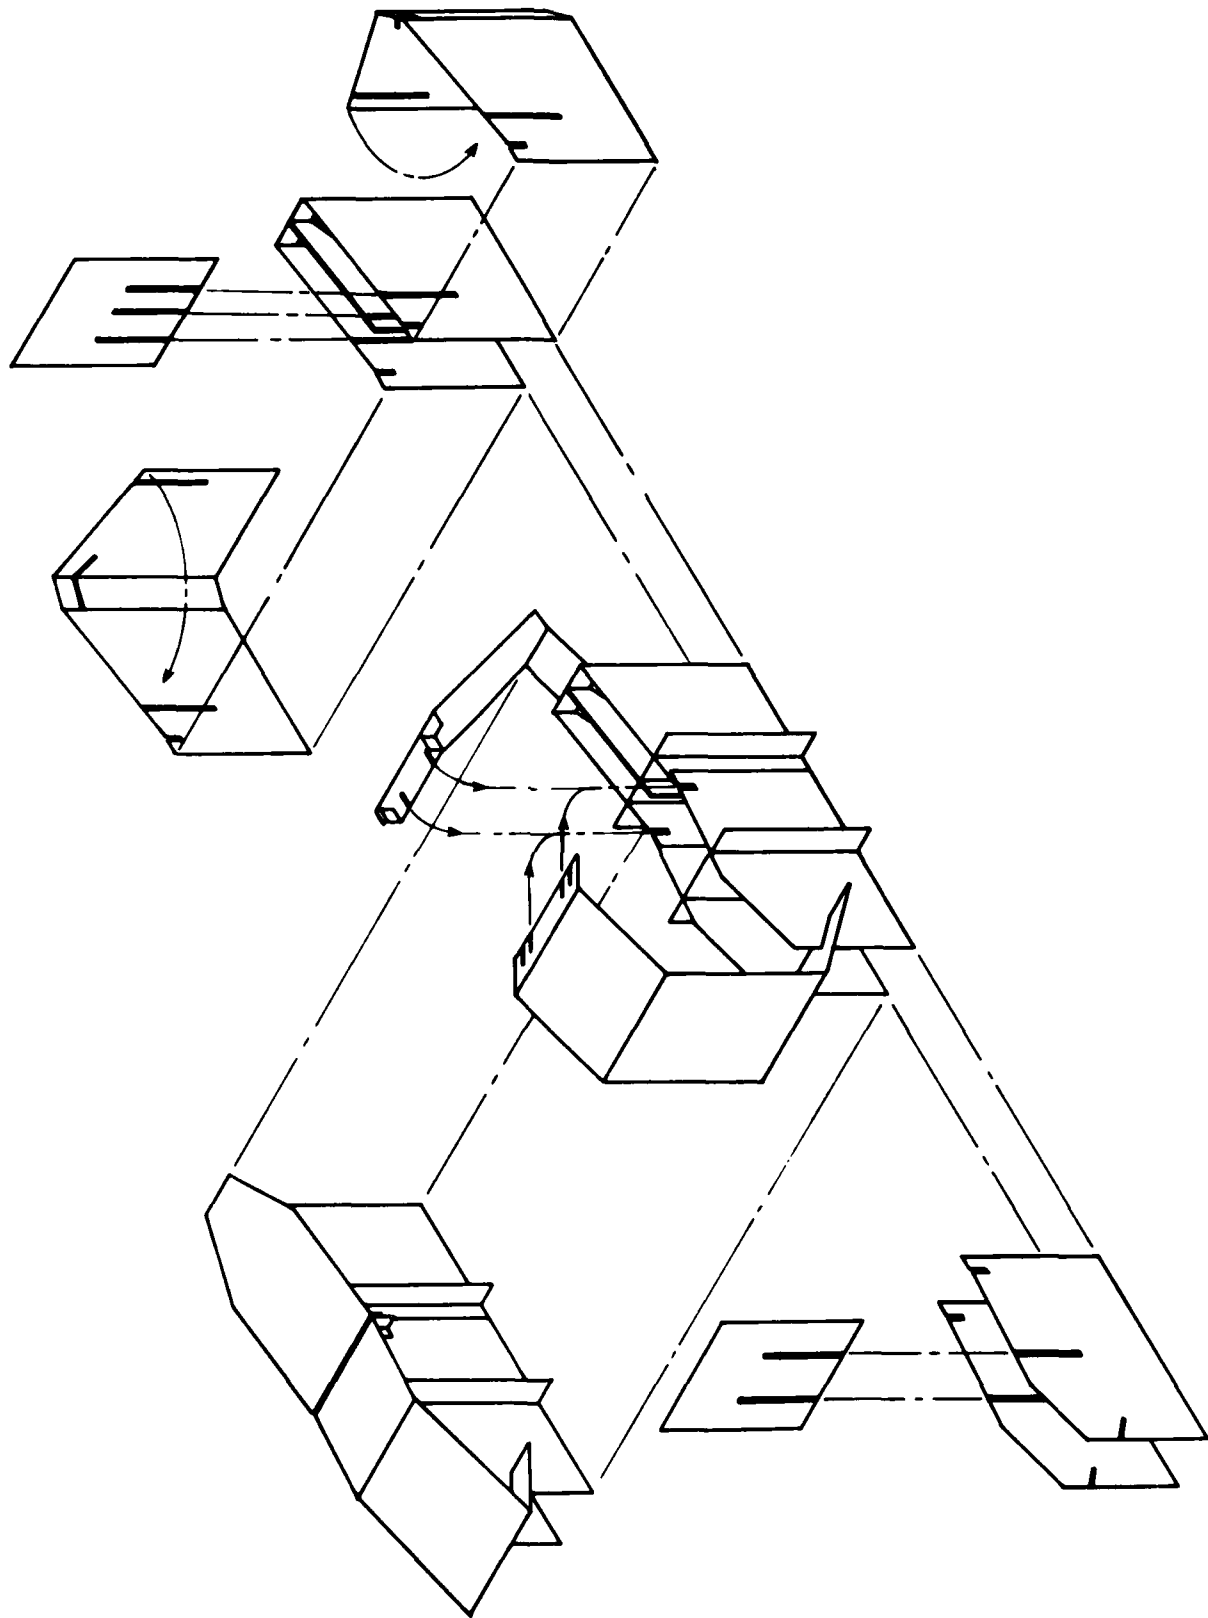


Figure 9. Chair assembly (reclining position).

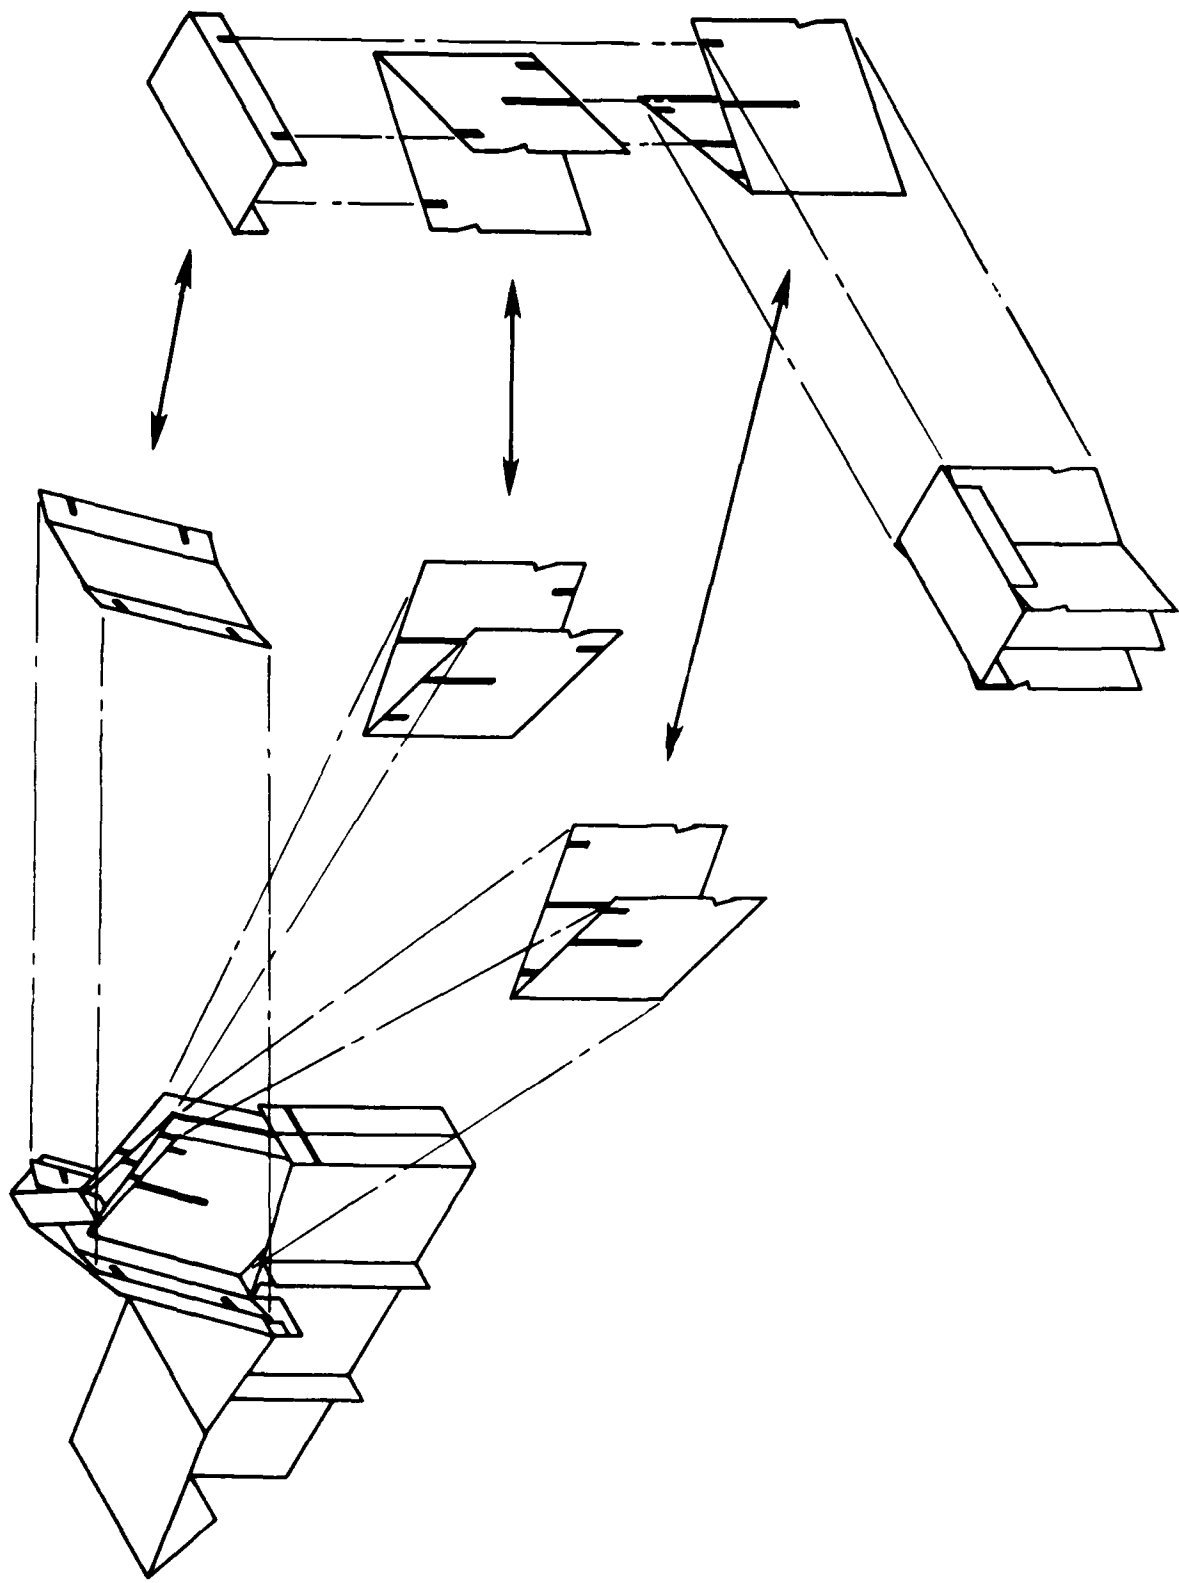


Figure 10. Stool and chair assembly (upright position).

UNCLASSIFIED

SECURITY CLASSIFICATION OF THIS PAGE (When Data Entered)

REPORT DOCUMENTATION PAGE		READ INSTRUCTIONS BEFORE COMPLETING FORM
1. REPORT NUMBER	2. GOVT ACCESSION NO. <b>A128 862</b>	3. RECIPIENT'S CATALOG NUMBER
4. TITLE (and Subtitle) ADJUSTABLE CARDBOARD DENTAL CHAIR AND STOOL		5. TYPE OF REPORT & PERIOD COVERED
		6. PERFORMING ORG. REPORT NUMBER NDRI-PR 83-04
7. AUTHOR(s) R. BAYCAR, F. AKER, A. SEROWSKI, and G. BAILEY		8. CONTRACT OR GRANT NUMBER(s)
9. PERFORMING ORGANIZATION NAME AND ADDRESS Naval Dental Research Institute Naval Base, Building 1-H Great Lakes, Illinois 60088		10. P. A. 4AM ELEMENT, PROJECT, TASK & WORK UNIT NUMBERS MO9: 02.0001
11. CONTROLLING OFFICE NAME AND ADDRESS Naval Medical Research and Development Command National Naval Medical Center Bethesda, MD 20814		12. R ATE FEB 1983
14. MONITORING AGENCY NAME & ADDRESS (if different from Controlling Office) Commander, Naval Medical Command Navy Department Washington, D. C. 20372		13. NUMBER OF PAGES 8
		15. SECURITY CLASS. (of this report) <b>UNCLASSIFIED</b>
16. DISTRIBUTION STATEMENT (of this Report) This document has been approved for public release; distribution unlimited.		15a. DECLASSIFICATION/DOWNGRADING SCHEDULE
17. DISTRIBUTION STATEMENT (of the abstract entered in Block 20, if different from Report) This document has been approved for public release; distribution unlimited.		
18. SUPPLEMENTARY NOTES		
19. KEY WORDS (Continue on reverse side if necessary and identify by block number) Dentistry Dental equipment Transportable Materials		
20. ABSTRACT (Continue on reverse side if necessary and identify by block number) A lightweight cardboard dental chair and stool has been designed and constructed for use in portable dental treatment. The chair is adjustable from the prone to the sitting position. All components disassemble into a compact package for storage and transportation.		

DD FORM 1473  
1 JAN 73

EDITION OF 1 NOV 68 IS OBSOLETE


S/N 0102-LF-014-6601

UNCLASSIFIED

SECURITY CLASSIFICATION OF THIS PAGE (When Data Entered)

UNCLASSIFIED

SECURITY CLASSIFICATION OF THIS PAGE (When Data Entered)



5 N 0102-LF-014-6601

UNCLASSIFIED

SECURITY CLASSIFICATION OF THIS PAGE(When Data Entered)

END

FILMED

6-83

DTIC