

AD-A141 167

A RODENT WATER DISPENSING SYSTEM FOR USE IN HYPOBARIC  
CHAMBERS(U) ARMY RESEARCH INST OF ENVIRONMENTAL  
MEDICINE NATICK MA J A DEVINE MAR 84 USARIEM-T-3/84


1/1

UNCLASSIFIED

F/G 14/2

NL



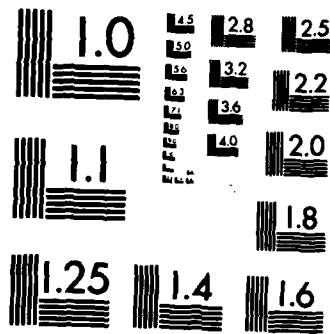

MICROCOPY RESOLUTION TEST CHART  
NATIONAL BUREAU OF STANDARDS-1963-A

12

AD \_\_\_\_\_

AD-A141 167

REPORT NO. T3/84

**A RODENT WATER DISPENSING SYSTEM  
FOR USE IN HYPOBARIC CHAMBERS**

**US ARMY RESEARCH INSTITUTE  
OF  
ENVIRONMENTAL MEDICINE  
Natick, Massachusetts**

DTIC FILE COPY

**MARCH 1984**



RELECTS  
MAY 1 7 1984

Approved for public release; distribution unlimited.



**UNITED STATES ARMY  
MEDICAL RESEARCH & DEVELOPMENT COMMAND**

84 05 16 046

The findings in this report are not to be construed as an official Department of the Army position, unless so designated by other authorized documents.

#### DTIC AVAILABILITY NOTICE

Qualified requesters may obtain copies of this report from Commander, Defense Technical Information Center (DTIC) (formerly DDC), Cameron Station, Alexandria, Virginia 22314.

#### DISPOSITION INSTRUCTIONS

Destroy this report when no longer needed.  
Do not return to the originator.

unclassified

SECURITY CLASSIFICATION OF THIS PAGE (When Data Entered)

REPORT DOCUMENTATION PAGE		READ INSTRUCTIONS BEFORE COMPLETING FORM
1. REPORT NUMBER T3/84	2. GOVT ACCESSION NO. AD-A141167	3. RECIPIENT'S CATALOG NUMBER
4. TITLE (and Subtitle) A Rodent Water Dispensing System for Use in Hypobaric Chambers		5. TYPE OF REPORT & PERIOD COVERED
		6. PERFORMING ORG. REPORT NUMBER
7. AUTHOR(s) James A. Devine		8. CONTRACT OR GRANT NUMBER(s)
9. PERFORMING ORGANIZATION NAME AND ADDRESS US Army Rsch Institute of Environmental Medicine Natick, MA 01760		10. PROGRAM ELEMENT, PROJECT, TASK AREA & WORK UNIT NUMBERS 3M161102BS10 44682101002
11. CONTROLLING OFFICE NAME AND ADDRESS Same as 9		12. REPORT DATE March 1984
		13. NUMBER OF PAGES
14. MONITORING AGENCY NAME & ADDRESS (if different from Controlling Office)		15. SECURITY CLASS. (of this report) unclassified
		15a. DECLASSIFICATION/DOWNGRADING SCHEDULE
16. DISTRIBUTION STATEMENT (of this Report) Unlimited		
17. DISTRIBUTION STATEMENT (of the abstract entered in Block 20, if different from Report)		
18. SUPPLEMENTARY NOTES		
19. KEY WORDS (Continue on reverse side if necessary and identify by block number) hypobaric chamber, water dispensing system, water loss, water consumption		
20. ABSTRACT (Continue on reverse side if necessary and identify by block number) A water dispensing system for rodents has been developed for use in chronic research studies involving hypobaric chambers. The system removes an existing problem that has restricted long-term animal exposures due to limitations inherent in the typical water supply bottles. The bottle design used in previous systems makes it susceptible to leakage whenever the water surface tension is disturbed. This disturbance occurs when water or room temperatures change, when animals are drinking, or more dramatically when the barometric pressure changes during ascents to altitude. Exposed water on the chamber floor may produce secondary health and		

DD FORM 1 JAN 73 1473

EDITION OF 1 NOV 65 IS OBSOLETE

unclassified

SECURITY CLASSIFICATION OF THIS PAGE (When Data Entered)

~~UNCLASSIFIED~~

SECURITY CLASSIFICATION OF THIS PAGE(When Data Entered)

environmental concerns. Daily returns to sea level to replenish drinking water and clean the chamber become the only available solution but add a complicating research variable. With the present water dispensing system, water may be replenished on-line for indefinite operations; water is available to rodent ad libitum, independent of the pressure differential without leakage; the system is insensitive to water pressure and malfunctions to mineral deposits; the amount of water consumed can be measured; and medications, drug, and vitamins may be administered.

UNCL A

SECURITY CLASSIFICATION OF THIS PAGE(When Data Entered)



## INTRODUCTION

One of the single most critical factors in limiting chronic hypobaric research studies with rodents is the limitations inherent in the typical water supply bottles. A rodent water dispensing bottle cannot be inverted without spillage. Additional water loss occurs when the air expands inside the bottle as water warms up to room temperatures or from temperature variations in the room itself. The reason is traceable to the bottle design where static pressure at the nozzle holds the water inside. This external pressure is in delicate balance with the negative pressure of the air space at the top of the fluid. A small disturbance can disrupt this surface tension equilibrium resulting in water loss. This happens when the bottle is jarred, the animal breaks the surface tension when drinking and/or the ambient barometric pressure changes with sufficient amplitude. The latter problem is magnified when water bottles are used for animal research studies conducted at low barometric pressure in hypobaric chambers. Large amounts of water are lost when the air pocket at the top of the bottle expands (increased volume) as the air pressure around the bottle decreases during ascents to altitude. Water loss also occurs due to minor oscillations under the finest of pressure control ( $\pm 1$  mmHg) and could account for significant losses when coupled with other disturbances such as animal feeding and nocturnal activities.

Exposed water on the chamber floor induces secondary health and environmental concerns and adds to the difficulties of conducting chronic



simulated altitude research studies. Daily returns to sea level to replenish drinking water and to clean the chamber become the only available solution but add a complicating variable.

In view of the water bottle limitations as described above, the automatic water drinking system represents a significant technological breakthrough. In removing the long-time problem that restricted chronic research studies, the water-dispensing system represents the following achievements: water may be replenished on-line for indefinite operations; water is available to the rodent ad libitum independent of the pressure differential without leakage; the system is insensitive to water pressure and malfunctions due to mineral deposits the amount of water consumed can be measured and medications, drugs and vitamins may be administered. The following text will explain the technological aspects of those achievements.

#### SYSTEM DESCRIPTION

The water supply container (Travenol Intravenous Bottle, I.V.) is located externally to the hypobaric simulator so replacement units may be installed without interrupting an ongoing study (Fig. 1). Toggle shut-off supply and vent (equalizing) valves isolate the bottle from the facility during replacement. It is possible to estimate animal water consumption because the bottle is graduated (0-1000 ml, in increments of 50 ml). Water is gravity-fed because the vent line equalizes the air space above

the fluid with the chamber pressure. The tubing (Imperial Eastman, Type 44P, Poly-flo) is not subject to embrittlement or swelling, has excellent resistance to flexural fatigue and can withstand a 200 psi pressure.


Bulkhead liquid/air tight connectors (Lapp, Model SL-7) provide uninterrupted feed-through for the poly-flow tubing (Fig. 2). A neoprene compression gland fits tightly around the tubing and effects a seal when the domed nut is threaded over the top of the tapered (collet) sleeve. The collet design accommodates various size tubing (.90 in - .265 in).

An automatic pivoting stem drinking valve (Edstrom, Model PV1035T) dispenses fluid to the rodent on demand (Fig. 3). When the animal drinks, the stem pivots on one side of its head which allows the other side to lift off the "O" ring and flex the diaphragm. Water then flows from the supply line, through the center of the "O" ring to the animal. As soon as the stem is released, the diaphragm closes the valve, stopping the flow of water. Since the stem pivots, it is like the use of a lever for lifting a heavy load. This allows a greater force to be exerted against the seal and yet little effort is required by the animal to obtain water. The entire system is insensitive to pressure changes since the valve may be operated with pressure differentials as high as 60 psi or as a gravity feed line. The drinking valve is connected to the animal cage with a Swagelock (Series "QC") quick-connect fitting. The automatic double-end shut-off minimizes pressure loss and fluid spillage during the push or pull operation used to connect or disconnect units. The quick-connect

fitting allows the cages to be removed for cleaning without loss of water from the system.

#### CONCLUSION

The water dispensing system for rodents in hypobaric chambers provides the potential for a no-loss infinite supply of water, permitting uninterrupted chronic research studies in hypobaric facilities. Other undesirable health and environmental problems caused by uncontrolled water losses have been eliminated. Water is available to the animal ad libitum, and there is no loss due to water or atmospheric pressure differentials. Cleaner cages, a cleaner chamber interior, a means of estimating water consumption, and the administration of medications are additional virtues of the water dispensing system.

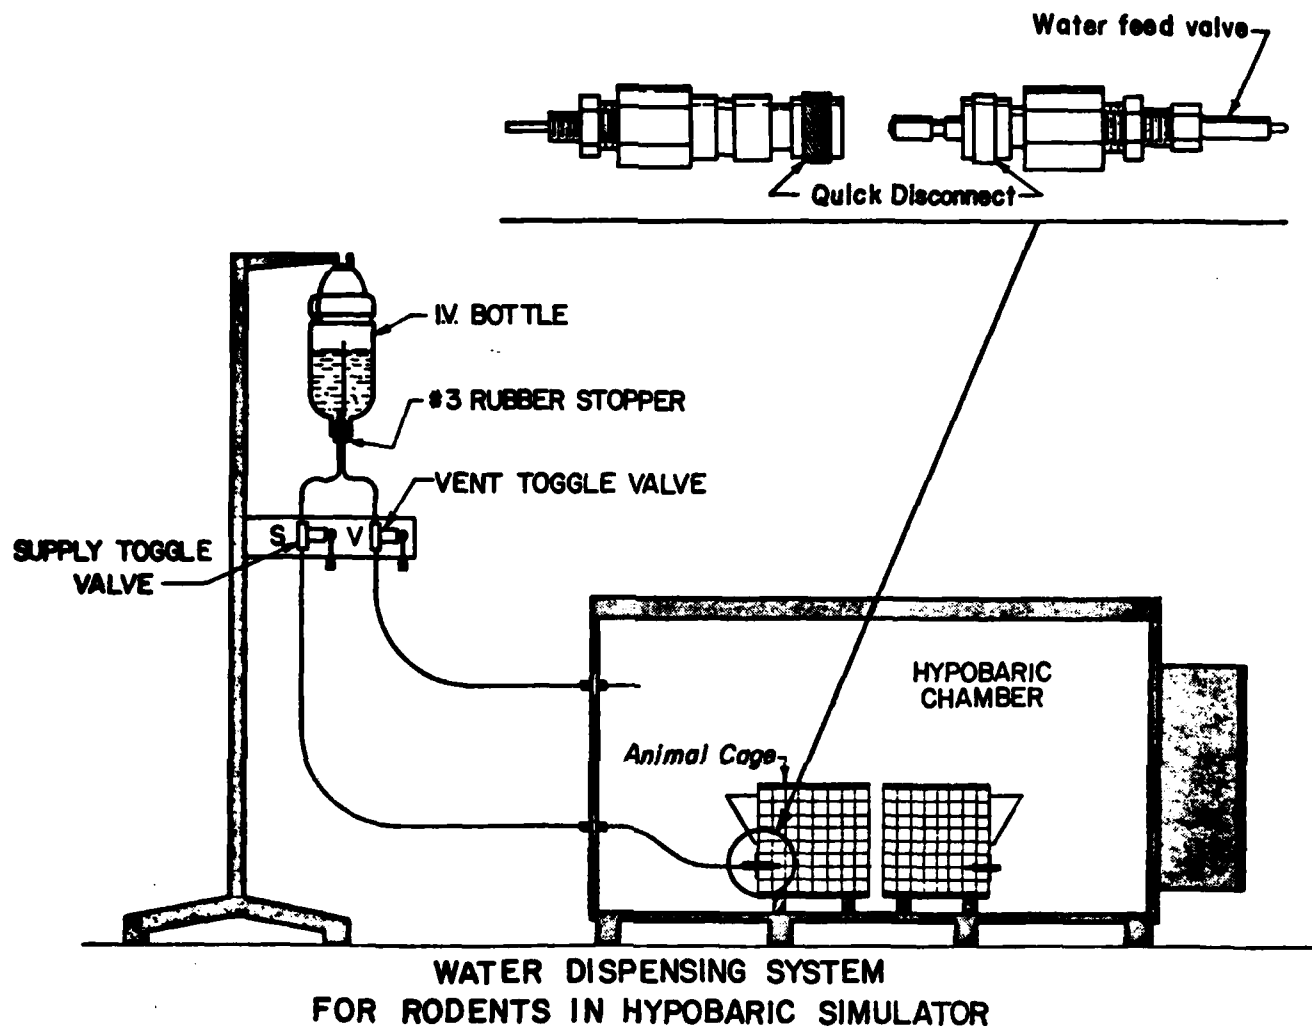

**Fig. 1.** Composite view of the water dispensing system with magnified view of the quick disconnect fitting containing the water feed valve.


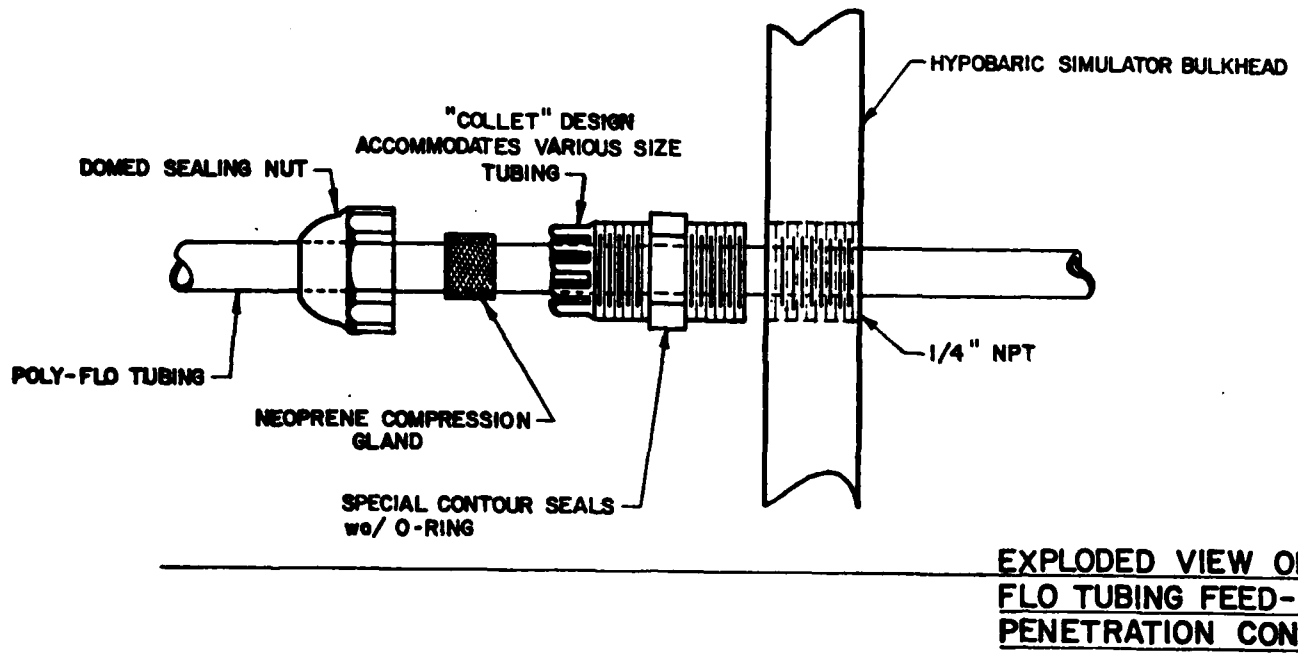


Fig. 2. Exploded view of the air-tight bulkhead connector used as a feed-through for the water supply tubing.

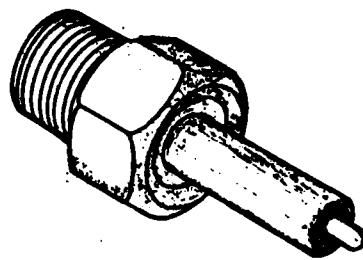

PIVOTING STEM DRINKING VALVE

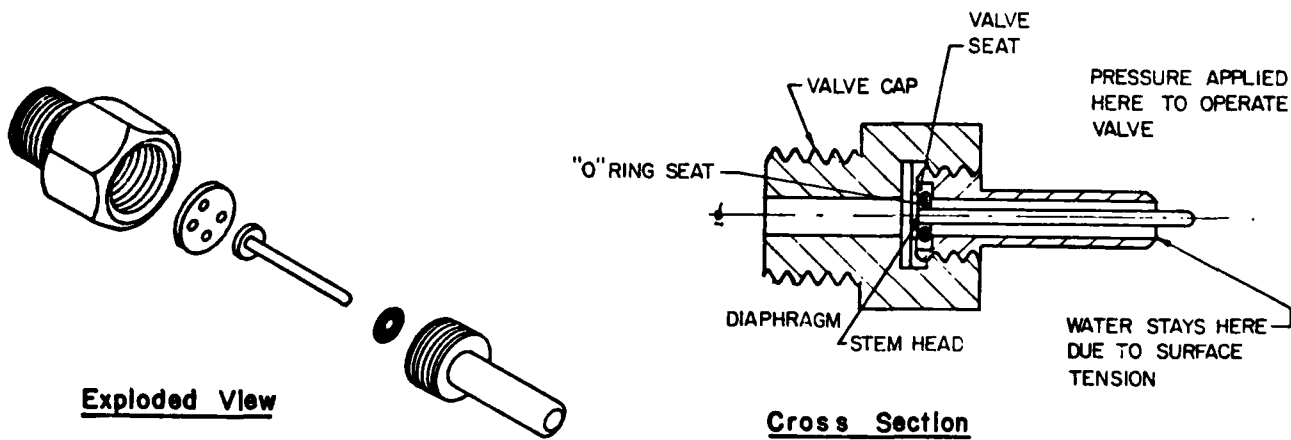


Fig. 3. Exploded and cross sectional views of the pivoting stem drinking valve.

DISTRIBUTION LIST

2 Copies to:

Commander  
US Army Medical Research and Development Command  
SGRD-RMS  
Fort Detrick  
Frederick, MD 21701

12 Copies to:

Defense Technical Information Center  
ATTN: DTIC-DDA  
Alexandria, VA 22314

1 Copy to:

Commandant  
Academy of Health Sciences, US Army  
ATTN: AHS-COM  
Fort Sam Houston, TX 78234

1 Copy to:

Dir of Biol & Med Sciences Division  
Office of Naval Research  
800 N. Quincy Street  
Arlington, VA 22217

1 Copy to:

CO, Naval Medical R&D Command  
National Naval Medical Center  
Bethesda, MD 20014

1 Copy to:

HQ AFMSC/SGPA  
Brooks AFB, TX 78235

1 Copy to:

Director of Defense Research and Engineering  
ATTN: Assistant Director (Environment and Life Sciences)  
Washington, DC 20301

REPRODUCED

FILMED

1954

DANIC