

1a. REPORT SECURITY CLASSIFICATION Unclassified		1b. RESTRICTIVE MARKINGS	
2a. SECURITY CLASSIFICATION AUTHORITY 2		3. DISTRIBUTION/AVAILABILITY OF REPORT Approved for public release; distribution is unlimited.	
AD-A232 715		5. MONITORING ORGANIZATION REPORT NUMBER(S) AFOSR-TR- 91 0091	
6a. NAME OF FUNDING/SPONSORING ORGANIZATION Arizona State University	6b. OFFICE SYMBOL (If applicable)	7a. NAME OF MONITORING ORGANIZATION AFOSR/NA	
6c. ADDRESS (City, State, and ZIP Code) Dept. of Mechanical and Aerospace Engineering Tempe, AZ 85287-6106		7b. ADDRESS (City, State, and ZIP Code) Building 410, Bolling AFB DC 20332-6448	
8a. NAME OF FUNDING/SPONSORING ORGANIZATION AFOSR/NA	8b. OFFICE SYMBOL (If applicable) NA	9. PROCUREMENT INSTRUMENT IDENTIFICATION NUMBER AFOSR 84-0187	
8c. ADDRESS (City, State, and ZIP Code) Building 410, Bolling AFB DC 20332-6448		10. SOURCE OF FUNDING NUMBERS	
		PROGRAM ELEMENT NO. 61102F	PROJECT NO. 2308
		TASK NO. A3	WORK UNIT ACCESSION NO.
11. TITLE (Include Security Classification) (U) Optimal Scaling of the Inverse Fraunhofer Diffraction Particle Sizing Problem: Analytic Eigenfunction Expansions.			
12. PERSONAL AUTHOR(S) E. Dan Hirleman			
13a. TYPE OF REPORT Paper reprint	13b. TIME COVERED FROM N/A TO N/A	14. DATE OF REPORT (Year, Month, Day) April 1989	15. PAGE COUNT 8
16. SUPPLEMENTARY NOTATION			
17. COSATI CODES		18. SUBJECT TERMS (Continue on reverse if necessary and identify by block number)	
FIELD	GROUP	Particle Sizing, Droplet Sizing, Sprays, Light Scattering, Multiple Scattering, optical diagnostics, optical sensors	
20	05		
21	02		
19. ABSTRACT (Continue on reverse if necessary and identify by block number)		Accession For	
See reverse		NTIS GRA&I <input checked="" type="checkbox"/>	
		DTIC TAB <input type="checkbox"/>	
		Unannounced <input type="checkbox"/>	
		Justification <input type="checkbox"/>	
		By _____	
		Distribution/	
		Availability Codes	
		Dist	Avail and/or Special
		A-1	
20. DISTRIBUTION/AVAILABILITY OF ABSTRACT <input checked="" type="checkbox"/> UNCLASSIFIED/UNLIMITED <input type="checkbox"/> SAME AS RPT <input checked="" type="checkbox"/> DTIC USERS		21. ABSTRACT SECURITY CLASSIFICATION Unclassified	
22a. NAME OF RESPONSIBLE INDIVIDUAL Julian M Tishkoff		22b. TELEPHONE (Include Area Code) (202) 767-4935	22c. OFFICE SYMBOL AFOSR/NA

DTIC ELECTE D
S MAR 12 1991

QUALITY INSPECTED
3

E. D. Hirtleman

Mechanical and Aerospace Engineering, Arizona State University, Tempe, Arizona

Optimal Scaling of the Inverse Fraunhofer Diffraction Particle Sizing Problem:
Analytic Eigenfunction Expansions

Abstract

There are many possible strategies for sampling the near-forward scattering pattern produced by a field of large particles and for subsequently solving the inverse problem in order to obtain an estimate of the particle size distribution. In a previous paper (*Part. Char.* Vol. 5, pp. 128-133, 1988) an optimally scaled formulation of the problem was derived based on consideration of condition numbers of the linear system obtained through numerical quadrature of the governing Fredholm integral equation. Here we consider "scaling" of the problem to involve selection of the parameters under control of the instrument designer (e.g. the number, angular positions, and aperture geometries of the detectors and the number, positions, and widths or weighting functions of the discrete size classes). Since the many numerical/analytical schemes for solving for the size distribution given a finite number of scattering measurements are fundamentally very similar, optimal scaling of the problem will improve the performance of the instrument regardless of the selected computational inversion algorithm.

In this paper we consider the analytic eigenfunction expansion method of solving the inverse Fraunhofer diffraction problem, and in particular how the scaling strategy affects the inversions. The eigenfunctions and associated eigenvalues for the diffraction problem (assuming infinite support) are derived in terms of two (variable) scaling parameters which describe the detector geometry and the size class configurations. It is shown that the rate of decrease of the eigenvalue spectrum with generalized frequency is minimized for the same scaling parameters ($a=2$, $b=2$) which optimized the condition numbers of the linear system. (A slower decrease in the eigenvalue spectrum indicates that the inversions will be less susceptible to corruption by noise, i.e. more stable). This optimal scaling study indicates, as was the case for the condition number analysis of the discrete linear system, that the particle size distribution solution should be on an area basis as $n(D)D^2$ and the scattering measurements should provide $i(\theta)\theta^2$.

E. D. Hirleman

Mechanical and Aerospace Engineering, Arizona State University, Tempe, Arizona

Optimal Scaling of the Inverse Fraunhofer Diffraction Particle Sizing Problem:
Analytic Eigenfunction Expansions

In a previous paper Hirleman [1] formulated the integral equation governing the inverse Fraunhofer diffraction particle sizing problem as follows:

$$i_a(\theta) = \int_0^{\infty} [I_{inc} \lambda^2 / 4\pi^2] [J_1^2(\alpha\theta) / (\alpha^{b-2}\theta^{2-a})] n_b(\alpha) d\alpha \quad (1)$$

where: $i(\theta)$ is the scattering intensity (W/sr) at a small forward angle θ ; I_{inc} is the irradiance (W/m²) of the incident beam (assumed uniform); α is the nondimensional particle size parameter equal to the particle circumference divided by the wavelength λ of the incident radiation ($\pi D/\lambda$); D is the particle diameter; $n(\alpha)$ is an unnormalized particle frequency distribution such that $n(\alpha)d\alpha$ is the number of optically-sampled particles in the optical beam with sizes between α and $\alpha + d\alpha$; J_1 is a Bessel function of first kind and first order; and a and b are constants where:

$$i_a(\theta) = i(\theta)\theta^a \quad (2)$$

$$n_b(\alpha) = n(\alpha)\alpha^b \quad (3)$$

Equation (1) assumes that Fraunhofer diffraction theory adequately describes the scattered light signature for the angles θ of interest and that multiple scattering is negligible. The diffraction assumption is satisfied generally when the angles θ are small, the particles are large compared to the wavelength, and the refractive index of the particles relative to the surroundings is not very close to unity. Finally, Eq. (1) neglects coherent scattering effects, i.e., assumes a very large number of randomly positioned particles are optically sampled. Now the scaling of the problem, which is the under auspices of the instrument designer, involves selection of parameters a and b and the number and orientations of detectors where measurements of $i_a(\theta)$ will be obtained. The measurements are used in the inverse problem, i.e. solving for $n_b(\alpha)$ in Eq. (1) using measured $i_a(\theta)$. Writing Eq. (1) in a more general integral equation form:

$$i_a(\theta) = I_{inc} \lambda^2 / 4\pi^2 \int_0^{\infty} k(\alpha, \theta) n_b(\alpha) d\alpha \quad (4)$$

where $k(\alpha, \theta)$ is the kernel of the integral equation and by inspection of Eq. (1):

$$k(\alpha, \theta) = J_1^2(\alpha\theta) / (\alpha^{b-2}\theta^{2-a}) \quad (5)$$

Now McWhirter and Pike [2] formulated a solution scheme to Fredholm integral equations such as Eqs. (1) and (4) which applies for cases where the kernel function $k(\alpha, \theta)$ is a function of only the product of the two variables, i.e. $k = k(\alpha\theta)$. With this requirement we see from Eq. (5) that:

$$2 - a = b - 2 \quad (6)$$

or:

$$a + b = 4 \quad (7)$$

and we have lost one degree of freedom in scaling the problem as a and b are no longer independent. Equation (7) is the same condition for which the linear system produced by numerical quadrature of Eq. (1) takes the Toeplitz form as discussed by Hirleman [1]. If we define a new independent scaling parameter δ as:

$$\delta \equiv 2 - a = b - 2 \quad (8)$$

Then Eq. (1) becomes:

$$i_{2,\delta}(\theta) = I_{inc} \lambda^2 / 4\pi^2 \int_0^{\infty} k_{\delta}(\alpha\theta) n_{\delta+2}(\alpha) d\alpha \quad (9)$$

where:

$$k_{\delta}(\alpha\theta) = J_1^2(\alpha\theta) / (\alpha\theta)^{\delta} \quad (10)$$

The eigenfunctions ψ_{ω} and associated eigenvalues λ_{ω} of the kernel, if they exist, are defined by:

$$\lambda_{\omega} \psi_{\omega}(\theta) = \int_0^{\infty} k(\alpha\theta) \psi_{\omega}(\alpha) d\alpha \quad (11)$$

where ω is a continuous generalized frequency. Thus any components of the solution function $n_b(\alpha)$ which can be expressed in terms of the eigenfunctions ψ_{ω} of k will be passed through the integral operator intact but scaled by the associated eigenvalue λ_{ω} . In that case the inversion of the integral equation would be performed by expanding the measured scattering signature $i_{2,\delta}(\theta)$ in a series of the eigenfunctions. The eigenfunction components with significant amplitudes would then be used to synthesize the solution function after scaling by the appropriate eigenvalues. Now if the following integral of the kernel k is bounded:

$$\int_0^{\infty} |k(x)| x^{-1/2} dx < \infty \quad (12)$$

then a continuum of real eigenfunctions exist and have been found using Mellin transforms by McWhirter and Pike [2] as:

$$\psi_{\omega}^{+}(\theta) = \text{Re}[\phi_{\omega}(\theta)] \quad (13)$$

$$\psi_{\omega}^{-}(\theta) = \text{Im}[\phi_{\omega}(\theta)] \quad (14)$$

where the corresponding real eigenvalues are:

$$\lambda_{\omega}^{\pm} = \pm |K((1/2) + i\omega)| \quad (15)$$

and where the Mellin transform $K(s)$ of $k(x)$ is defined by:

$$K(s) \equiv \int_0^{\infty} x^{s-1} k(x) dx \quad (16)$$

and:

$$\phi_{\omega}(\theta) = \frac{\theta^{-(1/2)-i\omega} \sqrt{K((1/2) + i\omega)}}{\sqrt{(\pi |K((1/2) + i\omega)|)}} \quad (17)$$

It is also sufficient to consider only $\omega > 0$ as pointed out by McWhirter and Pike [2] and Viera and Box [3].

Now we will need to obtain the Mellin transform defined in Eq. (16) of the kernel family of Eq. (10) as:

$$\begin{aligned} K_{\delta}(s) &= \int_0^{\infty} x^{s-1} J_1^2(x) / x^{\delta} \\ &= \frac{(1/2)^{\delta-s} \Gamma(\delta+1-s) \Gamma(1-(\delta/2)+(s/2))}{2 \Gamma^2(1+(\delta/2)-(s/2)) \Gamma(2+(\delta/2)-(s/2))} \end{aligned} \quad (18)$$

We can then calculate the eigenvalue spectrum from Eq. (17) which requires:

$$K_{\delta}((1/2)+i\omega) = \frac{(1/2)^{\delta-(1/2)-i\omega} \Gamma(\delta+(1/2)-i\omega) \Gamma((5/4)-(\delta/2)+(i\omega/2))}{\Gamma^2((3/4)+(\delta/2)-(i\omega/2)) \Gamma((7/4)+(\delta/2)-(i\omega/2))} \quad (19)$$

which, for $\delta=2$ simplifies to Eq. (3.3) of Bertero and Pike [4].

Before going further we must also consider the values of δ for which the kernel k_δ of Eq. (10) satisfies Eq. (12). Substituting k_δ for k in Eq. (12) results in the condition:

$$\int_0^{\infty} J_1^2(x) x^{-(1/2)-\delta} dx < \infty \quad (20)$$

Convergence of this integral requires that $3 > (-1/2-\delta) > 0$ or:

$$2.5 > \delta > -0.5 \quad (21)$$

For this paper we consider integer values for δ of 0, 1, and 2 which give physically meaningful properties to the functions $i_{2,\delta}$ and $n_{\delta+2}$ as shown in Table I.

δ	$i_{2,\delta}(\theta)$	Detector	$n_{\delta+2}(\alpha)$	Form of $n_{\delta+2}(\alpha)$
2	$i(\theta)$	Linear Array	$\alpha^4 n(\alpha)$	
1	$i(\theta)\theta$	Constant Δr Rings	$\alpha^3 n(\alpha)$	Volume distribution
0	$i(\theta)\theta^2$	Log-scaled Rings	$\alpha^2 n(\alpha)$	Area distribution

Now an indication of the quality of the scaling of an inverse problem is the rate at which the eigenvalues roll off with increasing frequency ω . This is true because the solution to Eq. (9) based on eigenfunction expansions will be:

$$n_{\delta+2}(\alpha) = \int_0^{\infty} n_{\delta,\omega}^+ \psi_{\omega}^+(\alpha) d\omega + \int_0^{\infty} n_{\delta,\omega}^- \psi_{\omega}^-(\alpha) d\omega \quad (22)$$

where:

$$n_{\delta,\omega}^{\pm} = i_{\delta,\omega}^{\pm} / \lambda_{\omega}^{\pm} \quad (23)$$

and:

$$i_{\delta,\omega}^{\pm} = \int_0^{\infty} i_{2-\delta}(\theta) \psi_{\omega}^{\pm}(\theta) d\theta \quad (24)$$

It can be seen from Eq. (23) that as the eigenvalues $\lambda_{\omega}^{\pm} \rightarrow 0$, the $n_{\delta,\omega}^{\pm}$ and therefore the solution grows without bound. The illconditioned nature of the problem would then be manifested

as small perturbations in $i_{\delta,\omega}^{\pm}$, for example due to measurement errors in $i_{2-\delta}(\theta)$, would be magnified greatly at frequencies ω where the λ_{ω}^{\pm} are small. For that reason it is necessary to truncate the integrations in Eq. (22) at some finite value ω_{\max} of the generalized frequency. In that case we approximate the solution as:

$$n\delta+2(\alpha) \equiv \int_0^{\omega_{\max}} n_{\delta,\omega}^{+} \psi_{\omega}^{+}(\theta) d\omega + \int_0^{\omega_{\max}} n_{\delta,\omega}^{-} \psi_{\omega}^{-}(\theta) d\omega \quad (25)$$

In that case, components of $n\delta+2(\alpha)$ at frequencies above ω_{\max} are inaccessible to the experiment.

Now there is a tradeoff between a desire to make ω_{\max} as large as possible in order to minimize the truncation error in Eq. (25) but at the same time keep the solution stable by not including frequencies with small eigenvalues. For that reason the behavior of the eigenvalue spectrum, shown in Fig. 1, is very important. For the possible values $\delta = 0, 1, 2$ the optimal value is clearly $\delta = 0$ which gives the slowest rolloff of λ_{ω}^{\pm} . The value $\delta = 0$ corresponds to $a = b = 2$, that is a solution on a particle area basis using log-scaled ring detectors. This result is identical to that obtained by Hirleman [1] using a condition number analysis on the linear system produced by numerical quadrature of Eq. (9).

The asymptotic behavior of the eigenvalue spectrum is interesting as well, and taking the limit of Eq. (19) as $\omega \rightarrow \infty$ and using Eq. (15) we obtain:

$$\lim_{\omega \rightarrow \infty} \lambda_{\omega}^{\pm} = \omega^{-\delta-1} \quad (26)$$

Again, the value of $\delta = 0$ is the best of the those considered, where in the limit of large ω the eigenvalues are proportional to ω^{-1} .

Some Comments on Instrument Design

It is clear from the previous analysis that the parameter δ , and in turn the instrument scaling parameters a and b , control the nature of the numerical inversion based on eigenfunction expansions. Thus the stability, the information content, and other measures of the performance of an inverse scattering solution based on analytic eigenfunctions is determined by the selection of parameters a and b . This has also shown to be the case for inversion of the linear system produced by numerical quadrature of Eq. (9), and it is expected to hold for a singular function expansion [3,5] as well. It is crucial, then, to understand constraints on the values of a and b which might be implemented in practice. Now an underlying assumption governing the validity of the condition number as a measure of inversion stability[1] and of the scheme proposed here for truncating the eigenfunction series approximation using a noise-based criterion is that of white noise. If, for example, the noise produced by a detector were constant per unit area of active detector surface, then the white noise assumption would only be true for $a = 0$ as pointed out by Bertero and Pike

[4,5]. This forces the instrument (for a product kernel or Toeplitz matrix form) to $b = 4$ and, in turn, $\delta = 2$. Clearly it would be better to have the freedom to select a detector geometry based on optimizing the expected numerical performance of the inverse problem and force the detector to conform rather than vice versa.

One possible approach is to use the optical system shown in Fig. 2 as developed by Hirleman and Dellenback [6], where the detector area (noise-producing) does not depend on the collection aperture for the discrete detection angles θ . The optical system of Fig. 2 uses a transmission-mode spatial light modulator to create programmable mosaic arrays (of arbitrary shape) of detector openings which pass selected portions of the scattering signature on through to the field lens and single detector. While the parallel, simultaneous detection capabilities are lost with a system as in Fig. 2, the potential for intelligent, programmable detector arrays overrides that disadvantage.

Acknowledgements

This research was sponsored by the Air Force Office of Scientific Research, Air Force Systems Command, USAF, under Grant Number AFOSR-84-0187, Dr. Julian Tishkoff, program manager. The U.S. Government is authorized to reproduce and distribute reprints for Governmental purposes notwithstanding any copyright notation thereon.

References

1. E. D. Hirleman, "Optimal Scaling for Fraunhofer Diffraction Particle Sizing Instruments," *Particle Characterization*, Vol. 4, pp. 128-133 (1988).
2. J. G. McWhirter and E. R. Pike. "On the Numerical Inversion of the Laplace Transform and Similar Fredholm Integral Equations of the First Kind", *J. Phys. A: Math. Gen.*, Vol. 11, pp. 1729-1745 (1978).
3. G. Viera and M. A. Box. "Information Content Analysis of Aerosol Remote-sensing Experiments Using Singular Function Theory. 1: Extinction Measurements", *Applied Optics*, Vol. 26, pp. 1312-1327, (1987).
4. M. Bertero and E. R. Pike. "Particle Size Distributions from Fraunhofer Diffraction I. An Analytic Eigenfunction Approach", *Optica Acta*, Vol. 30, pp. 1043-1049 (1983).
5. M. Bertero, P. Boccacci, C. De Mol and E. R. Pike. "Particle Size Distributions from Fraunhofer Diffraction", pp. 99-105 in *Optical Particle Sizing, Theory and Practice*, G. Gouesbet and G. Grehan, eds., Plenum, New York, 1988.
6. E. D. Hirleman and P. A. Dellenback, "Adaptive Fraunhofer Diffraction Particle Sizing Instrument using a Spatial Light Modulator", pp. 217-220 in *Spatial Light Modulators and Applications*, V. 8, Optical Society of America, Washington, D.C., 1988. Under review by *Applied Optics*.

Nomenclature

a	instrument scaling parameter (nondimensional) for particle size distribution function basis
b	instrument scaling parameter (nondimensional) for scattering intensity moment
D	particle diameter (m)
$i(\theta)$	scattering intensity (W/sr) at angle θ
I_{inc}	incident irradiance (W/m ²)
J_1	Bessel function of first kind and first order
$k(\alpha, \theta)$	general kernel function for the integral equation
$k(\alpha\theta)$	product-form of the kernel k
K	Mellin transform of the kernel function k
α	particle size parameter, $\pi D/\lambda$
δ	instrument scaling parameter (nondimensional) which arises when k is a product kernel.
θ	scattering angle measured from the optical axis
λ_ω	eigenvalue corresponding to frequency ω
ψ_ω	eigenfunction for the kernel of the integral equation
ω	generalized frequency

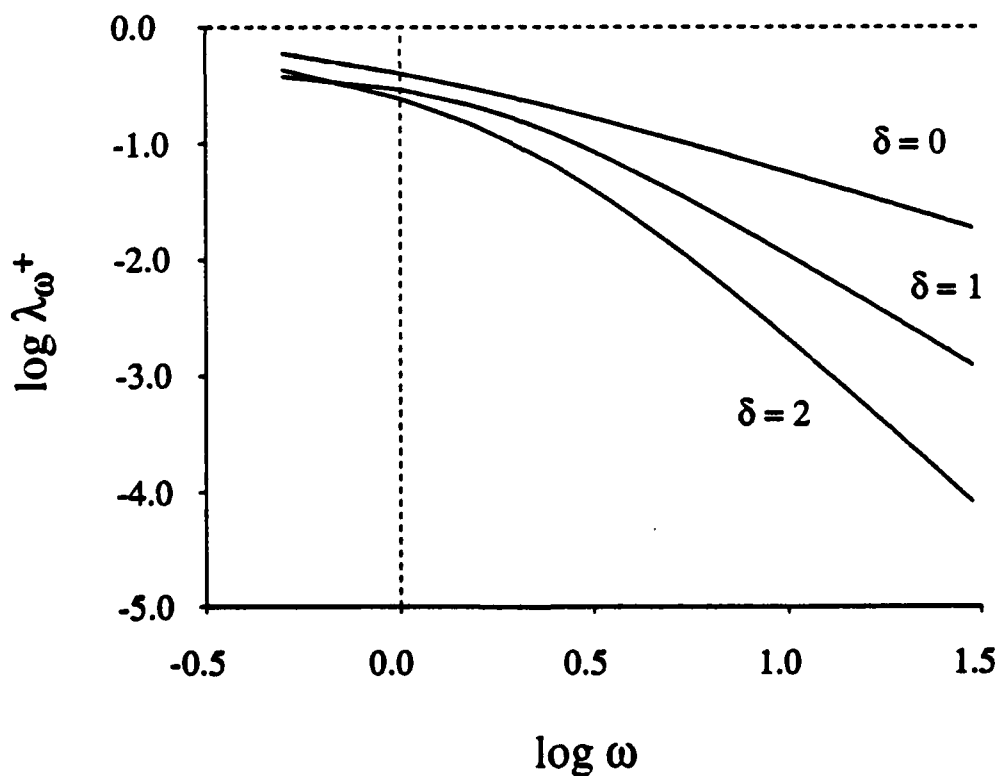


Figure 1. Plot of the eigenvalue spectrum λ_ω^+ of the Fraunhofer diffraction integral equation for the kernel described by Eq. (19). The spectra for three values of the scaling parameter δ are shown. The asymptotic behavior of the curves are described by Eq. (26).

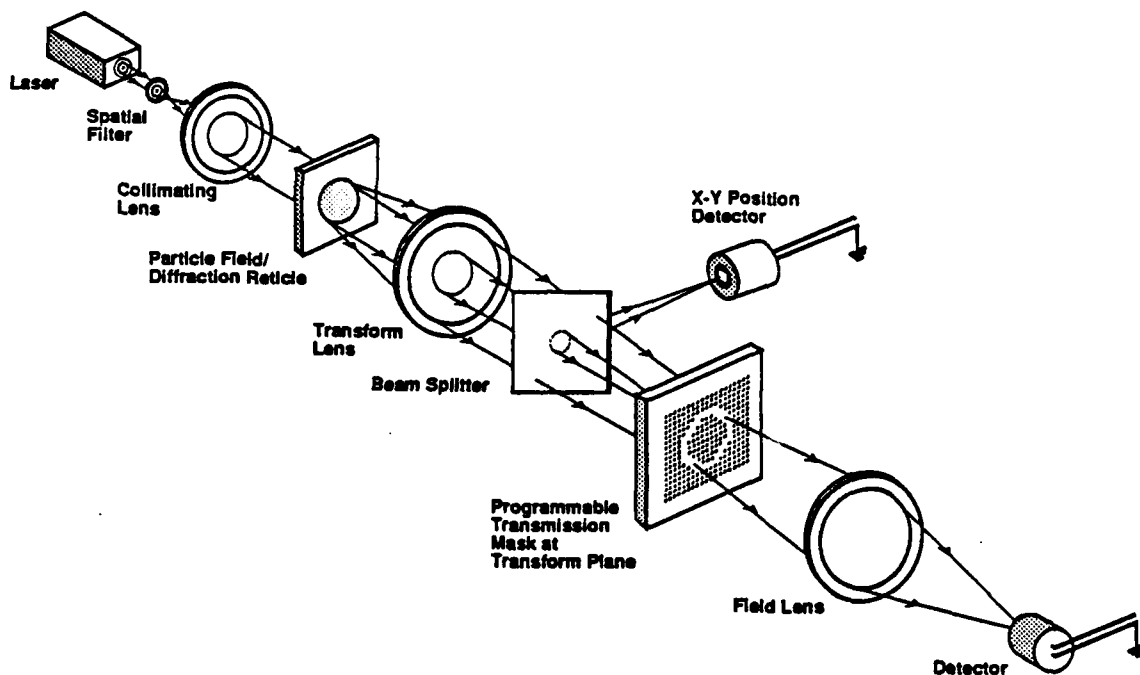


Figure 2. Schematic of a laser diffraction particle sizing instrument where a spatial light modulator operated as a programmable transmission mask has been included to provide for on-line, adaptive configuration of the detector collection apertures. Annular ring openings are created in the SLM at the transform plane by setting the pixels to transmit or block the incident polarized light. The rings are created concentric with the optical axis as measured in real-time by the x-y position detector shown. The field lens collects all light passing through the SLM and passes it the the detector, and the system is sequenced through a set of rings.