

# Report Documentation Page

*Form Approved*  
*OMB No. 0704-0188*

Public reporting burden for the collection of information is estimated to average 1 hour per response, including the time for reviewing instructions, searching existing data sources, gathering and maintaining the data needed, and completing and reviewing the collection of information. Send comments regarding this burden estimate or any other aspect of this collection of information, including suggestions for reducing this burden, to Washington Headquarters Services, Directorate for Information Operations and Reports, 1215 Jefferson Davis Highway, Suite 1204, Arlington VA 22202-4302. Respondents should be aware that notwithstanding any other provision of law, no person shall be subject to a penalty for failing to comply with a collection of information if it does not display a currently valid OMB control number.

1. REPORT DATE <b>2008</b>	2. REPORT TYPE	3. DATES COVERED <b>00-00-2008 to 00-00-2008</b>			
4. TITLE AND SUBTITLE <b>Inlaid Carbon Nanofiber Nanoelectrode Array as Highly Efficient Dielectrophoresis Device for Bacteria Trapping</b>		5a. CONTRACT NUMBER			
		5b. GRANT NUMBER			
		5c. PROGRAM ELEMENT NUMBER			
6. AUTHOR(S)		5d. PROJECT NUMBER			
		5e. TASK NUMBER			
		5f. WORK UNIT NUMBER			
7. PERFORMING ORGANIZATION NAME(S) AND ADDRESS(ES) <b>Department of Chemistry, Kansas State University, Manhattan, KS, 66506</b>		8. PERFORMING ORGANIZATION REPORT NUMBER			
9. SPONSORING/MONITORING AGENCY NAME(S) AND ADDRESS(ES)		10. SPONSOR/MONITOR'S ACRONYM(S)			
		11. SPONSOR/MONITOR'S REPORT NUMBER(S)			
12. DISTRIBUTION/AVAILABILITY STATEMENT <b>Approved for public release; distribution unlimited</b>					
13. SUPPLEMENTARY NOTES <b>See also ADM002137. Proceedings of the 2008 IEEE International Conference on Nanotechnology (8th) Held in Arlington, TX on August 18-21, 2008. U.S. Government or Federal Rights License</b>					
14. ABSTRACT					
15. SUBJECT TERMS					
16. SECURITY CLASSIFICATION OF:			17. LIMITATION OF ABSTRACT <b>Same as Report (SAR)</b>	18. NUMBER OF PAGES <b>2</b>	19a. NAME OF RESPONSIBLE PERSON
a. REPORT <b>unclassified</b>	b. ABSTRACT <b>unclassified</b>	c. THIS PAGE <b>unclassified</b>			

# Inlaid Carbon Nanofiber Nanoelectrode Array as Highly Efficient Dielectrophoresis Device for Bacteria Trapping

Jun Li<sup>1</sup>, Member, IEEE, Prabhu U. Arumugam<sup>2</sup>, Hua Chen<sup>2</sup>, Alan Cassell<sup>3</sup>

<sup>1</sup> Department of Chemistry, Kansas State University, Manhattan, KS 66506, USA. E-mail: junli@ksu.edu

<sup>2</sup> ELORET, NASA Ames Research Center, Moffett Field, CA 94035, E-mail: prabhu.u.arumugam@nasa.gov, hchen@nasa.gov

<sup>3</sup> University Affiliated Research Center, University of California-Santa Cruz, and NASA Ames Research Center, Moffett Field, CA 94035, acassell@nasa.gov

**Abstract**-Dielectrophoresis (DEP) is an effective microelectronic technique for trapping and manipulating biological particles in a microfluidic environment, which relies on the highly asymmetric electric field gradient created by the microelectrodes. Here we demonstrate an AC DEP technique for single-bacteria trapping using nanoelectrode arrays (NEAs) in a “points-and-lid” configuration. The NEA is based on vertically aligned carbon nanofibers (CNFs) embedded in SiO<sub>2</sub> matrix. The miniaturization of the electrode size provides a highly focused electric field with the gradient enhanced by several orders of magnitude. Finite element modeling indicated that the pDEP force using such NEA-based devices can be increased by over 100 times. Experiments indicated that the bacteria can be trapped instantaneously on to the exposed CNF tip with an AC voltage of  $\sim 3 V_{pp}$ . In most cases, a single *E. coli* bacterium is trapped at a single CNF site due to the screening effect. Such nano-DEP device allows the integration of millions of nanoelectrodes deterministically in lab-on-a-chip devices that can be used for effective cell manipulating and concentration.

## BACKGROUND

Cell manipulation is the first critical step in single-cell analysis. Microscale DEP technique<sup>1</sup> has been widely used for a large number of cells because the electric field distributions can be precisely controlled by lithographically patterned electrodes in microfluidics down to single-cell resolution, i.e. at 1-50 microns. To capture smaller particles (bacteria, viruses, prions, etc.), it requires further miniaturization of electrode dimensions. One possible solution is to use one-dimensional nanostructures. It is known that the high aspect ratio nanostructures such as carbon nanotubes (CNTs) improve field emission due to the strong enhancement of electric field strength at the sharp tip<sup>2</sup>. Recently, Torma et al.<sup>3</sup> observed extremely high field gradients ( $\sim 10^{23} V^2 m^{-3}$ ) with multi-walled CNT DEP for DNA trapping. But it lacks a precise placement and control of electrode dimensions, much needed for biological studies. Here, we investigated the use of NEAs fabricated by inlaying vertically aligned CNFs (50-200 nm dia.) in SiO<sub>2</sub> matrix as a DEP trap in aqueous solution.

DEP is based on the polarization of particles in a non-uniform electric field.<sup>4</sup> The time-average DEP force on the particle in a sinusoidal field is  $\langle F_{dep}(t) \rangle = \pi \epsilon_m R^3 \text{Re} [K(\omega)] \cdot \nabla |E(r)|^2$ , where  $\epsilon_m$  is the permittivity of the medium, R is the

particle radius,  $\text{Re}[K(\omega)]$  is the real part of complex Clausius-Mossotti factor  $K=(\epsilon_p-\epsilon_m)/(\epsilon_p+2\epsilon_m)$  defined by the angular frequency ( $\omega$ ) dependent complex permittivity of the medium ( $\epsilon_m$ ) and particle ( $\epsilon_p$ ). For  $\epsilon_p > \epsilon_m$ , as in the case of cells and viruses,  $\text{Re}[K(\omega)]$  is positive and particles move toward higher electric field, resulting in positive DEP (pDEP). The magnitude is proportional to  $\nabla |E(r)|^2$ , determined by the electrode geometry and voltage. For a nanoelectrode (NE),  $\nabla |E(r)|^2$  can be increased over 100 times, generating a much stronger DEP force. The large pDEP force is able to counter Stokes drag force in a high-velocity laminar microfluidic flow and effectively traps *E. coli* at individual NEs.

## MATERIALS AND METHODS

The NEAs based on inlaid vertical CNF arrays were fabricated following the similar methods reported before<sup>5</sup>: A microscope was used to observe the *E. coli* movement through an ITO electrode (as shown in Fig. 1a). The typical CNF array consists of 50-200 nm diameter and  $\sim 5 \mu m$  long fibers with an average spacing of  $\sim 400$  nm. Each CNF was vertically aligned and freestanding on the surface. We controlled the condition so that only a small number of CNFs are exposed with an average spacing more than 1 micron. In a few samples (such as Fig. 1b), e-beam lithography was used to pattern the Ni catalysts into a well-separated hexagonal array of nanodots ( $\sim 100$  nm in dia.) which produced an array of individual CNFs. A layer of SU-8 was spin-coated and UV exposed to form the microfluidic channel and bound the NEA chip with the ITO counter electrode.

## CURRENT RESULTS

The two-dimensional (2D) finite element modeling of pDEP trapping at a linear array of 12 CNF NEs at  $26 V_{pp}$  and a flow velocity of 10 mm/s is shown in Fig. 2. Particles of 1  $\mu m$  in diameter are injected at various heights simulating *E. coli*. The trajectories show that all particles injected below 12  $\mu m$  height are trapped while others (including those near the 20  $\mu m$  high ceiling) are deflected downwards. The flow velocity (10 mm/s) is much higher than those in micro- “points-and-lid” device (0.1-0.5 mm/s)<sup>6</sup> and interdigitated device (0.04-2 mm/s)<sup>7</sup>,

reflecting the higher trapping efficiency. The  $E(r)^2$  map around a NE tip shows a maximum of  $\sim 1.2 \times 10^{14} \text{ V}^2 \text{ m}^{-2}$ , 200 times higher than that of the micro- “points-and-lid” device<sup>6</sup>. At 2 mm/s flow velocity, even 9  $V_{pp}$  can trap most of the particles.

The trapping of *E. coli* is measured by the integrated fluorescence intensity from stained *E. coli* by focusing at a  $\sim 0.25\text{-mm}^2$  area at the bottom of the channel with a dimension of  $500\mu\text{m}(\text{W}) \times 20\mu\text{m}(\text{H}) \times 2\text{cm}(\text{L})$  as shown in Fig. 3a. An *E. coli* suspension ( $\sim 1 \times 10^9/\text{ml}$ ) is continuously passed through the microchannel. The trap is turned on and off to observe how *E. coli* are captured and released from the NEA. The DEP voltage is varied between 0 to 9  $V_{pp}$  in a series of experiments. At a flow velocity of  $\sim 2\text{mm/s}$ , even 1  $V_{pp}$  initiates evident trapping. At  $V_{pp} > 3 \text{ V}$ , CNF NEs are able to generate strong DEP force to trap *E. coli* that instantaneously covered all exposed CNF tips.

Fluorescence images are taken before and after the 3  $V_{pp}$  is turned on. When the  $V_{pp}$  is off at the beginning (Fig. 3b), *E. coli* bacteria are floating in water and generate fuzzy stretched tracks. After a 3  $V_{pp}$  is turned on (Fig. 3c), bacteria are instantaneously snapped onto the exposed CNF tips, generating sharp bright spots while the extra bacteria are still floating. The trapped bacteria can be reversibly released when the  $V_{pp}$  is turned off.

In summary, we have demonstrated the use of embedded CNF NEA in trapping small bioparticles against strong hydrodynamic drag forces in a microfluidic channel. This new nano-DEP technique can be used either as a low-density array for registration and the study of single particles or a high-density array that is tailored as an active DEP filter for sorting, separating, and concentrating bioparticles. This approach of manipulating submicron bioparticles by highly focused strong electrical fields at NEAs, promises new capabilities for cell biology research and the development of highly integrated biochips for environmental and security monitoring.


#### ACKNOWLEDGMENT

This work was supported by NASA Ames Research Center. We thank Dr. Meyya Meyyappan for his support and discussion.


#### REFERENCES

[1] J. Voldman, "Electrical forces for microscale cell manipulation," *Annu. Rev. Biomed. Eng.*, vol. 8, pp. 425-454, 2006.  
 [2] L. Nilsson, O. Groenig, C. Emmenegger, O. Kuettel, E. Schaller, L. Schlapbach, H. Kind, J.-M. Bonard, and K. Kern, "Scanning field emission from patterned carbon nanotube films," *Appl Phys Lett*, vol. 76, pp. 2071-2073, 2000.  
 [3] S. Tuukkanen, J. J. Toppari, A. Kuzyk, L. Hirviniemi, V. P. Hytonen, T. Ihalainen, and P. Torma, "Carbon nanotubes as electrodes for dielectrophoresis of DNA," *Nano Letters*, vol. 6, pp. 1339-1343, 2006.  
 [4] H. A. Pohl, *Dielectrophoresis: The behavior of neutral matter in nonuniform electric fields*. Great Britain: Cambridge Univ. Press, 1978.  
 [5] J. Li, J. E. Koehne, A. M. Cassell, H. Chen, H. T. Ng, Q. Ye, W. Fan, J. Han, and M. Meyyappan, "Inlaid multi-walled carbon nanotube nanoelectrode arrays for electroanalysis," *Electroanalysis*, vol. 17, pp. 15-27, Jan 2005.


[6] D. S. Gray, J. L. Tan, J. Voldman, and C. S. Chen, "Dielectrophoretic registration of living cells to a microelectrode array (vol 19, pg 1765, 2004)," *Biosensors & Bioelectronics*, vol. 19, pp. 1765-1774, 2004.  
 [7] H. Li, Y. Zheng, D. Akin, and R. Bashir, "Characterization and Modeling of a microfluidic dielectrophoresis filter for biological species.," *Microelectromech. Syst.*, vol. 14, pp. 103-112, 2005.

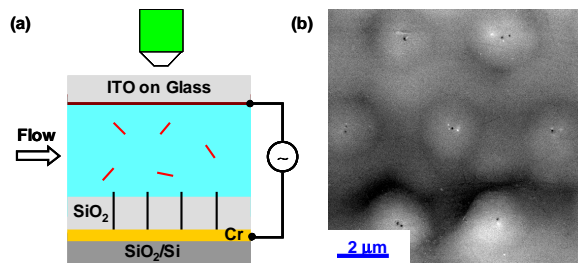

**Fig. 1** (a) The layout of the “points-and-lid” DEP device with a CNF NEA at the bottom and ITO counter electrode at the top of the microchannel. The electrodes are separated by a patterned SU-8 polymer, which also forms the seal for microchannel. (b) SEM image of the top view of an inlaid regular CNF NEA that was patterned by e-beam lithography.

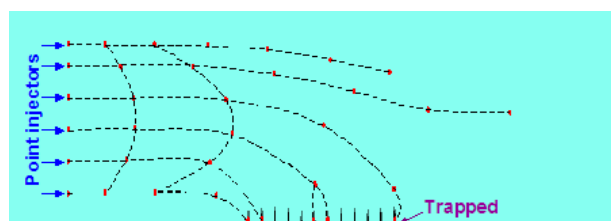

**Fig. 2** Modeling of pDEP trapping on CNF NE array. The dashed lines show the trajectories of 1- $\mu\text{m}$  dia. particles under the influence of Stokes drag force of a 10 mm/s flow and dielectrophoretic forces by an 10 MHz AC voltage of 26  $V_{pp}$ .

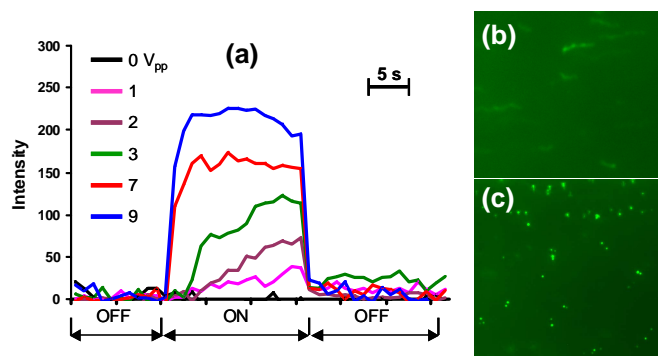

**Fig. 3** (a) Integrated epifluorescence intensity when the 1 MHz AC  $V_{pp}$  is switched on and off in a  $\sim 250 \mu\text{m/s}$  flow. (b) Epifluorescence images showing *E. coli* flowing through and trapped at CNF NEs before and after the  $V_{pp}$  is turned on.