

AD-A044 103 HARRY DIAMOND LABS ADELPHI MD

AN ASSEMBLY-LANGUAGE DIGITAL DIVISION COMPUTER PROGRAM FOR USE --ETC(U) SEP 77 C R HEIMBACH HDL-TM-77-20 UNCLASSIFIED NL | OF | ADA044103 END DATE FILMED

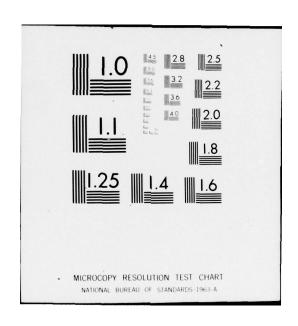

HDL-TM-77-70


MDA 044103



An Assembly-Language Digital Division
Computer Program for Use
in Proton-Recoil Spectroscopy

September 1977





U.S. Army Material Development and Readlacts Commend MARRY DIAMOND LABORATORIES Adolphi, Maryland 20703

POPULATED FOR PORCE PERENE; DUTTINGUTED UNLINTED

UNCLASSIFIED

SECURITY CLASSIFICATION OF THIS PAGE (When Data Entered)

REPORT DOCUMENTATION PAGE	READ INSTRUCTIONS BEFORE COMPLETING FORM
HDL-TM-77-20	N NO. 3. DECHE IENT'S CATALOG NUMBER
A. TITLE (and Substite) An Assembly-Language Digital Division	Technical Memorandum
Computer Program for Use in Proton-Reco Spectroscopy.	6. PERFORMING ORG. REPORT NUMBER
7. AUTHOR(e)	8. CONTRACT OR GRANT NUMBER(*)
Craig R. Heimbach	Pron: Al-7R000402A1A9
9. PERFORMING ORGANIZATION NAME AND ADDRESS	10. PROGRAM ELEMENT, PROJECT, TASK AREA & WORK UNIT NUMBERS
Harry Diamond Laboratories 2800 Powder Mill Road Adelphi, MD 20783	Program: 6.21.18.A
Adelphi, MD 20783 11. CONTROLLING OFFICE NAME AND ADDRESS U.S. Army Materiel Development and Readiness Command	September 277
Alexandria, VA 22333	16
14. MONITORING AGENCY NAME & ADDRESS(II different from Controlling Off	Unclassified
(13)12p.	15a. DECLASSIFICATION/DOWNGRADING SCHEDULE
17. DISTRIBUTION STATEMENT (of the abetract entered in Block 20, if different	ent from Repetit) DEPENDED 14 1977
HDL Project No.: X75721 DRCMS Code: 6121188750011	SEP
19. KEY WORDS (Continue on reverse side if necessary and identify by block no	umber)
Proton recoil	
Computer program Pulse-height division	
Computer program Pulse-height division 20. AD TRACT (Continue on reverse side if necessary and identity by block not a computer program has been modifi for an analog divider for a neutron-energy and identity by block not a neutron-energy and identity by block not a computer program has been modified to a neutron-energy and identity by block not a neutron-energy and	ed to circumvent the need ergy spectrometer in use at
Computer program Pulse-height division 20. ABOURACT (Continue on reverse side if recessary and identify by block now A computer program has been modifit for an analog divider for a neutron-ene the Harry Diamond Laboratories. The sp recoil system, and some division proces nate against gamma sensitivity of the g	ed to circumvent the need ergy spectrometer in use at pectrometer is a proton- es is necessary to discrimi- gas proton-recoil detectors.
Computer program Pulse-height division 20. AD TRACT (Continue an reverse stds # necessary and identify by block nu A computer program has been modifif for an analog divider for a neutron-ene the Harry Diamond Laboratories. The sp recoil system, and some division proces	ted to circumvent the need ergy spectrometer in use at pectrometer is a protonss is necessary to discrimigas proton-recoil detectors. Achine language for the

163050

1/3

SECURITY CLASSIFICATION OF THIS PAGE(When Date Entered)

analyzes data. Coincident dual-parameter data (energies of recoiling protons and pulse rise times) are acquired by the program. The rise-time pulse-height distribution is divided by the energy distribution before storage in the computer memory. This normalization facilitates subtraction of the unwanted gamma sensitivity of the proton-recoil detectors, particularly at low neutron energies.

The elimination of the analog divider improves performance and simplifies the operation of the spectrometer.





CONTENTS

		Page				
1	INTRODUCTION	5				
2	METHOD OF GAMMA-RAY DISCRIMINATION	5				
3	DIFFICULTIES WITH METHOD	6				
4	METHOD OF SOLUTION	6				
5	ELECTRONIC MODIFICATIONS	6				
6	PROGRAM MODIFICATIONS	7				
	6.1 Description of Program	7				
	6.2 Explanation of Subroutines	8				
	6.3 Use of Program	8				
	6.4 Constraints on Method	8				
7	SUMMARY	9				
	LITERATURE CITED	9				
	DISTRIBUTION	15				
	APPENDIX ADIGITAL DIVIDE PROGRAM	11				
	FIGURES					
1	Distribution of neutron and gamma-ray pulses	5				
2	Dual-parameter data distribution 6					
3	Electronics with analog voltage division					
4	Electronics with digital voltage division					

1. INTRODUCTION

Harry Diamond Laboratories (HDL) is presently developing a capability for fast-neutron spectrometry. One method being pursued is the proton-recoil technique. ^{1,2,3} With this method, neutrons from a nuclear reactor penetrate a detector containing hydrogen or methane gas and collide with the protons. The protons recoil and create in the gas ion pairs that are collected by an applied electric field. The voltage pulses resulting from the collected ions are proportional to the energy of the protons. Pulse-height analysis of the voltage pulses allows the energy spectrum of the protons to be determined. The proton spectrum is then analyzed to provide the energy spectrum of the high-energy neutrons.

Any cause of ionization in the detector gas other than the protons is a source of noise. In particular, gamma rays that accompany the high-energy neutrons also ionize the gas. Voltage pulses that have gamma rays as their origin must be separated from those which are due to the neutrons.

2. METHOD OF GAMMA-RAY DISCRIMINATION

Usually, this separation of pulses is performed by pulse-shape discrimination. Because the protons have a greater specific ionization than Compton electrons that result from gamma interactions, they have shorter path lengths in the gas. Hence, their voltage pulses have shorter rise times than those due to the gamma rays.

Figure 1 illustrates the pulse-separation technique. Figure 1(a) shows the differences in pulse-height distributions from neutrons and gamma interactions. In figure 1(b), the separation is increased for the smaller pulse heights by use of specific ionization rather than rise time to distinguish between the neutronand gamma-ray-induced pulses. The specific ionization is obtained by dividing the rise time of each voltage pulse by its magnitude. The resulting dual-parameter distribution is pictured in figure 2.

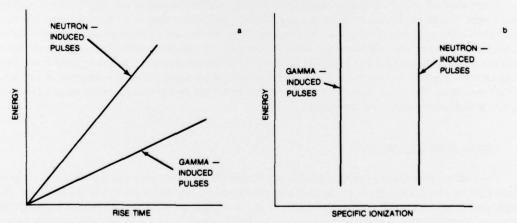


Figure 1. Distributions of neutron and gamma-ray pulses. Energy versus rise time (a) and energy versus specific ionization (b).

¹ E. F. Bennett and T. J. Yule, Techniques and Analyses of Fast-Reactor Neutron Spectroscopy with Proton-Recoil Proportional Counters, Argonne National Laboratory, ANL-7763 (1971).

E. F. Bennett, Nuclear Science Engineering, 27(1967), 16-27.

¹ Fast Neutron Physics, VI, Ch IIA, Interscience (1966).

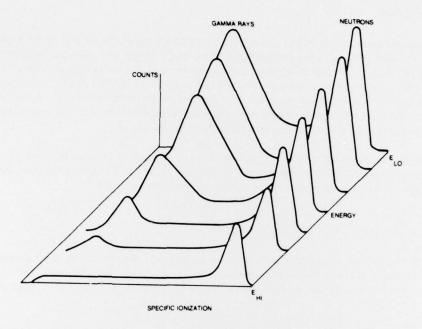


Figure 2. Dual-parameter data distribution.

3. DIFFICULTIES WITH METHOD

A key element of the gamma-ray separation technique is the division of rise-time pulses by voltage pulse height. The desired division can be accomplished by either an analog or a digital divider. However, experience with an analog divider was the principal emphasis for our need to develop a digital divide technique. In order to perform the analog division correctly, the rise-time and pulse-height signals had to enter the analog voltage divider in coincidence. Because of this requirement, the analog divider was very sensitive to fluctuations in time. It was also sensitive to variation in signal size or the presence of a dc level in the input signal. The elimination of the divider eliminates these problems and greatly reduces the time necessary to place the system into operation.

4. METHOD OF SOLUTION

The method developed to do this division was to modify the electronics and the computer program which control data acquisition from the proton-recoil detectors. The electronic modification is relatively simple and is described first. The modification of the computer program and background information necessary to operate the program and to interpret the results are discussed in the remainder of the report.

5. ELECTRONIC MODIFICATIONS

Originally, the electronics that couple the proton proportional counters (the detectors for the neutron spectrometer) through the ADC's (analog-to-digital converters) to the minicomputer were arranged as shown in figure 3. The signals from the proton-recoil counters were amplified to give a total amplitude

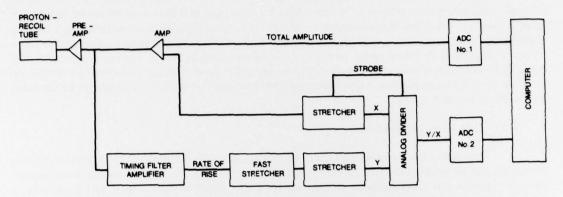


Figure 3. Electronics with analog voltage division.

pulse in one ADC. Such pulses are proportional to the energies of the recoiling protons. Simultaneous with this energy measurement, the timing-filter amplifier differentiates and amplifies the signals to give the rate of rise. These signals (energy and rate of rise) are fed in coincidence into the Y/X analog-voltage divider to produce the input to the second ADC, which forms the specific ionization axis of the dual-parameter array.

Since the ADC's and memory units are under control of a minicomputer, it is possible to have the alternative arrangement shown in figure 4. The total amplitude (energy) signal is the same as before, but since the Y/X division is now done digitally within the minicomputer, the second ADC accepts rate-of-rise information directly.

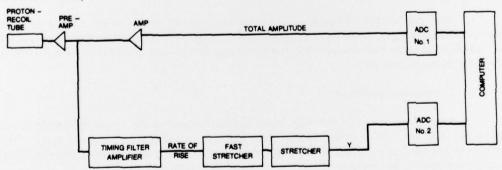


Figure 4. Electronics with digital voltage division.

6. PROGRAM MODIFICATIONS

6.1 Description of Program

The digital divide program is listed in appendix A. It is written in assembly language⁴ for the ND812 computer and is in the form of an overlay for the ND-1075-01, which is the dual-parameter data-acquisition program.⁵

^{*} Nuclear Data Incorporated, Software Instruction Manual, BASC-12 General Assembler, Palatine, IL (1962).

³ Nuclear Data Incorporated, Software Instruction Manual, ND4420 Single/Dual Parameter Monitor, Palatine, IL (1972).

The ND-1075-01 has a special subroutine which handles data coming from the ADC's. Normally, this subroutine polls the ADC's to collect X and Y input and then increments the appropriate point in memory. The digital divide modification leaves the X input unchanged, but modifies the Y input by dividing it by X. Then the appropriate point in memory is incremented. All the other routines of ND-1075-01 are unaffected, with the exception of the auto-experiment routines. These routines are changed only because the overlay had to be put somewhere in memory and the auto-experiment routines are rarely used for proton-recoil data acquisition. If one had to use these routines, the overlay would have to be moved to an unused portion of memory.

6.2 Explanation of Subroutines

The digital divide overlay consists of four subroutines: RSSAV, RSRES, NEW1, and NEW2. The subroutine RSSAV modifies the ADC handling routine to save the R and S registers so that these registers may be used by the other portions of the ND-1075-01. RSRES restores the R and S registers to whatever their original contents were before the ADC interrupt occurred. This is necessary because the R and S registers have meaning to portions of the 1075 program external to the ADC routines. Location FIRST also has to be saved and restored because the location of the patches eliminates the instruction that normally does this.

The routine NEW1 stores the results of the X-ADC for future reference. The routine NEW2 takes the results of the Y-ADC, multiplies by a scale factor FMP, divides by the X-ADC results, and then returns control to the ND-1075-01 program with the results in the K register. The ND-1075-01 uses the results in the K register as the Y input and increments the appropriate location in memory.

6.3 Use of Program

First, the ND-1075-01 program is loaded into fields 00 and 01 of the ND812 computer. A binary version of the digital divide program is overlaid on top of this in field 00 by the paper-tape loader. The multiplication factor FMP (location 7507, field 00) may be varied to move the Y/X result to the left or right on an oscilloscope display.

6.4 Constraints on Method

Precautions must be taken with digital division because of the size of the rate-of-rise pulses coming into ADC no. 2. With analog division, these pulses consisted of pulse height divided by rise time and were independent of pulse height. Therefore, the gain of the timing filter amplifier could be set to give adequate resolution at one energy and it was automatically adequate at all energies.

In the digital division arrangement, the pulses coming into ADC no. 2 are proportional to energy. One may set the timing filter amplifier to give adequate resolution in the middle of the energy range, but there are still problems at the extreme low and high ends of the energy range.

First, consider the low end of the energy range. The input to ADC no. 2 consists of small voltage pulses, which are digitized to only a few significant figures. This causes a loss of accuracy in the rise time, making the separation of gamma rays more difficult. Fortunately, sufficient accuracy may be achieved in the digital technique by increasing the resolution of ADC no. 2 from 256 divisions full scale, which was adequate with the analog division arrangement, to 4096.

Next, consider the high end of the energy range. The input pulses to ADC no. 2 grow larger with energy and may exceed the maximum signal capacity of the ADC. If this occurs, data will be lost. This data loss may be avoided by keeping the gain of the timing filter amplifier sufficiently low.

The operator must remember to set the resolution of ADC no. 2 to 4096. Since the overlay automatically interacts with the ND-1075-01, no further action on the part of the operator is necessary.

7. SUMMARY

An assembly-language computer program has been written which allows the electronic analog divider to be eliminated from the HDL proton-recoil spectroscopy system. This has the advantage of simplifying the electronics and greatly reducing the time necessary to set up the system. In order to use the program, the resolution of ADC no. 2 (the rise-time ADC) has to be increased to 4096 divisions and care must be taken to see that the rise-time signal does not grow beyond the capacity of ADC no. 2 before the energy signal grows beyond the capacity of its ADC.



LITERATURE CITED

- E. F. Bennett and T. J. Yule, Techniques and Analyses of Fast-Reactor Neutron Spectroscopy with Proton-Recoil Proportional Counters. Argonne National Laboratory, ANL-7763 (1971).
- 2. E. F. Bennett, Nuclear Science Engineering, 27(1967), 16-27.
- Fast Neutron Physics. VI, Ch IIA, Interscience (1966).
- Nuclear Data Incorporated, Software Instruction Manual, BASC-12 General Assembler, Palatine, IL (1962).
- Nuclear Data, Incorporated, Software Instruction Manual, ND4420 Single/Dual Parameter Monitor, Palatine, IL (1972).

APPENDIX A.—DIGITAL DIVIDE PROGRAM

This digital divide program is written in assembly language¹ for the ND812 computer. It is in the form of an overlay for the ND-1075-01, which is the dual-parameter data-acquisition program.²

0

SE 5353 = 1374 EXJK FMP = 7407 NEW1 = 7400 NE W2 = 7410NE WP - 7400 RSRES = 7440 - 7425 RSSAV RSTR = 7436 SSTR = 7437 = 7406 X ER 0000 A<A< A<B<\,< = < =))<=

(3,(<)<(G<

EX JK=1374 NE WP=7400

/NEWP LOCATES THE OVERLAY POSITION

/ THE FOLLOWING TWJMP'S ARE PATCHES INTO THE 1075 WHICH / DIRECT IT TO THE DIGITAL DIVIDE ROUTINES

/

0137

*0111

NE WI

0111	0600	TWJMP
0112	7425	RSSAV
		+0117
0117	0600	TWJMP
01 20	7440	RSRES
		*0136
0136	0600	TWJMP

7400

¹ Nuclear Data Incorporated, Software Instruction Manual, BASC-12 General Assembler, Palatine, IL (1962).

² Nuclear Data Incorporated, Software Instruction Manual, ND4420 Single/Dual Parameter Monitor, Palatine, IL (1972).

```
*0210
                    TWJMP
0210
     0600
0211
      7410
                    NEAS
                    *NEWP
/ UPON ENTERING NEWI, J CONTAINS THE VALUE OF THE X ADC.
/ THE EXJK. TWSTJ DO WHAT USED TO BE DONE BY THE 1075
/ WHERE THE TWJMP NEW! IS NOW LOCATED
                    STJ X
7400 5406 NEWI.
     1374
7401
                    EXJK
7402 0540
                    TWSTJ
     0175
                    0175
7403
                    TWJMP
7404
     0600
     0140
                    0140
                           /RETURN TO THE 1075
7405
7406
     0000 X.
7407 0400 FMP.
                   0400
                           NORMALIZATION FACTOR
/ NEW2 TAKES THE Y-ADC VALUE, MULTIPLIES BY THE SCALE FACTOR
/ FMP, DIVIDES BY THE X-ADC VALUE, AND STORS THE RESULT INTO
/ THE 1075 SO THAT THE APPROPRIATE DATA LOCATION MAY BE
/ INCREMENTED AND DISPLAYED
                           /K=Y AFTER
7410 1374 NEW2.
                   EXJK
    0540
                   TWSTJ
                            / SAVE J
7411
7412
     0175
                    0175
     5104J
7413
                    LDJ FMP
                            NORMALIZE Y
7414
     1000
                    MPY
7415
     5107 J
                   LDJ X
7416 1303
                   EX JRKS
7417
    1001
                    DIV
                           /Y/X
7420
    1374
                           /PUT IN K
                   EXJK
7421
     0500
                   TWLDJ
                            / RESTORE J
                   0175
7422
     0175
7423
     0600
                    TWJMP
7424
     2120
                    0212
                            /RETURN TO 1075
/ RSSAV SAVES THE CONTENTS OF THE R AND S REGISTERS
/ SO THAT R AND S MAY BE USED IN THE DIVIDE INSTRUCTION
/ FIRST MUST BE SAVED BECAUSE THE TWJMP RSSAV IS IN THE
/ LOCATION WHERE FIRST IS USUALLY SAVED
```

```
5000 RSSAV, LDJ FIRST
7425
7426
      0540
                    TWSTJ
                            /STORAGE LOCATION FOR FIRST IN ADC
7427
      0173
                    0173
7430 1302
                    LJKFR5
                            INTERRUPT
      5405
                    STJ RSTR
7431
                    TWSTK
7432 0550
7433
      7437
                    SSTR
                    TWJMP
7434
      0600
                            /RETURN TO 1075
      0113
                    0113
7435
7436
      0000 RSTR.
                    0
                            /STORAGE LOCATION FOR R
      0000 SSTR.
                            /STORAGE LOCATION FOR S
7437
                    0
/ RESTORE R AND S BEFORE LEAVING ADC INTERRUPT ROUTINE
7440
      5102 RSRES, LDJ RSTR
7441
      0510
                    TWLDK
7442
      7437
                    SSTR
7443
      1301
                    LRSFJK
7444
     1410
                    CLR FLAG
7445
     1450
                    CLR O
7446 0600
                    TWJMP
7447 0121
                    0121
SE 5353
        = 1374
EXJK
FMP
        = 7407
NEW1
        = 7400
NEWS
        = 7410
NEWP
        = 7400
RSRES
        = 7440
RSSAV
        - 7425
RSTR
        = 7436
SSTR
        = 7437
X
        = 7406
ER 0000
```

DISTRIBUTION

DEFENSE DOCUMENTATION CENTER CAMERON STATION, BUILDING 5 ALEXANDRIA, VA 22314 ATTN DDC-TCA (12 COPIES)

COMMANDER
USA RSCH & STD GP (EUR)
BOX 65
FPO NEW YORK 09510
ATTN LTC JAMES M. KENNEDY, JR.
CHIEF, PHYSICS & MATH BRANCH

COMMANDER
US ARMY MATERIEL DEVELOPMENT
& READINESS COMMAND
5001 EISENHOWER AVENUE
ALEXANDRIA, VA 22333
ATTN DRXAM-TL, HQ TECH LIBRARY
ATTN DRCDE-A, PROGRAM SUPPORT OFC

COMMANDER
US ARMY ARMAMENT MATERIEL
READINESS COMMAND
ROCK ISLAND ARSENAL
ROCK ISLAND, IL 61201
ATTN DRSAR-ASF, FUZE & MUNITIONS
SPT DIV

COMMANDER
USA MISSILE & MUNITIONS CENTER & SCHOOL
REDSTONE ARSENAL, AL 35809
ATTN ATSK-CTD-F

NAVAL TRAINING EQUIPMENT CENTER ORLANDO, FL 32813 ATTN TECHNICAL LIBRARY

ARGONNE NATIONAL LABORATORY 9700 SOUTH CASS AVE ARGONNE, IL 60439 ATTN ENGINEERING R&D

US DEPARTMENT OF COMMERCE
ASSISTANT SECRETARY FOR SCIENCE
& TECHNOLOGY
WASHINGTON, DC 20230

US DEPARTMENT OF COMMERCE NATIONAL BUREAU OF STANDARDS WASHINGTON, DC 20230

US ENERGY RESEARCH & DEVELOPMENT ADMINISTRATION WASHINGTON, DC 20545 ATTN DIV OF REACTOR RES & DEV

US ENERGY RESEARCH & DEVELOPMENT ADMINISTRATION TECHNICAL INFORMATION ORGANIZATION P.O. BOX 62 OAK RIDGE, TN 37830

DIRECTOR
ARMED FORCES RADIOBIOLOGY RESEARCH
INSTITUTE
DEFENSE NUCLEAR AGENCY
NATIONAL NAVAL MEDICAL CENTER
BETHESDA, MD 20014

DIRECTOR
DEFENSE ADVANCED RESEARCH
PROJECTS AGENCY
ARCHITECT BLDG
1400 WILSON BLVD
ARLINGTON, VA 22209
ATTN TECH INFO OFFICE

DIRECTOR
DEFENSE NUCLEAR AGENCY
WASHINGTON, DC 20305
ATTN PETER HAAS, DEP DIR,
SCIENTIFIC TECHNOLOGY
ATTN RADIATION DIRECTORATE

CHIEF
LIVERMORE DIVISION,
FIELD COMMAND, DNA
LAWRENCE LIVERMORE LABORATORY
P.O. BOX 808
LIVERMORE, CA 94550
ATTN H. KLAPPER

OFFICE, CHIEF OF RESEARCH, DEVELOPMENT & ACQUISITION DEPARTMENT OF THE ARMY WASHINGTON, DC 20310 ATTN DAMA-AR, RESEARCH PROGRAMS

PROJECT MANAGER, M60 TANKS
US ARMY MATERIEL DEV &
READINESS COMMAND
28150 DEQUINDRE
WARREN, MI 48092

COMMANDER
US ARMY NUCLEAR AGENCY
FORT BLISS, TX 79916
ATTN ATCN-W, WEAPONS EFFECTS DIV

COMMANDER
WHITE SANDS MISSILE RANGE, NM 88002
ATTN STEWS-ID, INSTRUMENTATION IDR
ATTN STEWS-IN, INFO OFFICE

DISTRIBUTION (Cont'd)

COMMANDER
EDGEWOOD ARSENAL
EDGEWOOD ARSENAL, MD 21010
ATTN SAREA-R, RES LABORATORIES

COMMANDER
US ARMY ARMAMENT RESEARCH &
DEVELOPMENT COMMAND
PICATINNY ARSENAL
DOVER, NJ 07801
ATTN DRDAR-ND-W, WEAPONS VULNERABILITY

COMMANDER
US ARMY ABERDEEN PROVING GROUND
ABERDEEN PROVING GROUND, MD 21005
ATTN STEAP-TL, TECH LIB
ATTN STEAP-MTM, METHODOLOGY & INSTR

OFFICE OF RESEARCH, DEVELOPMENT,
TEST & EVALUATION
DEPT OF THE NAVY
WASHINGTON, DC 20360
ATTN NOP-985, NUCLEAR ENERGY DIV

DIRECTOR
NAVAL RESEARCH LABORATORY
WASHINGTON, DC 20375
ATTN CODE 2620, LIBRARY
ATTN CODE 4000, RESEARCH DEPT
ATTN CODE 6620, RADIATION EFFECTS

COMMANDER AEROSPACE RESEARCH LABORATORIES WRIGHT-PATTERSON AFB, OH 45433

DIRECTOR
AF OFFICE OF SCIENTIFIC RESEARCH
1400 WILSON BLVD
ARLINGTON, VA 22209
ATTN DO, RES OPERATIONS

COMMANDER
AF WEAPONS LAB, AFSC
KIRTLAND AFB, NM 87117
ATTN SE, NUCLEAR SYS DIV

DIRECTOR
NASA
GODDARD SPACE FLIGHT CENTER
GREENBELT, MD 20771
ATTN 250, TECH INFO DIV

HARRY DIAMOND LABORATORIES ATTN RAMSDEN, JOHN J., LTC, COMMANDER/ FLYER, I.N./LANDIS, P.E./ SOMMER, H./OSWALD, R. B. ATTN CARTER, W.W., DR., TECHNICAL DIRECTOR/MARCUS, S.M. ATTN DANIEL, CHARLES D., JR., MG, COMMANDING GENERAL (ERADCOM) ATTN KIMMEL, S., PAO ATTN CHIEF, 0021 ATTN CHIEF, 0022 ATTN CHIEF, LAB 100 ATTN CHIEF, LAB 200 ATTN CHIEF, LAB 300 ATTN CHIEF, LAB 400 ATTN CHIEF, LAB 500 ATTN CHIEF, LAB 600

ATTN CHIEF, DIV 800
ATTN CHIEF, LAB 900
ATTN CHIEF, LAB 1000
ATTN RECORD COPY, BR 041
ATTN HDL LIBRARY (5 COPIES)
ATTN CHAIRMAN, EDITORIAL COMMITTEE
ATTN CHIEF, 047
ATTN TECH REPORTS, 013
ATTN PATENT LAW BRANCH, 071

ATTN CHIEF, DIV 700

ATTN GIDEP OFFICE, 741