

HDL-TM-92-5

April 1992



AD-A250 757



2

Double-Sided Wafer Alignment Techniques

by Timothy J. Mermagen
Bruce R. Geil

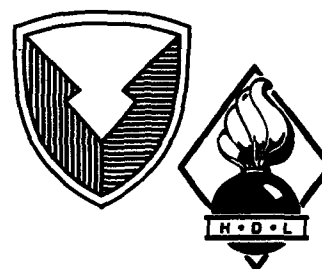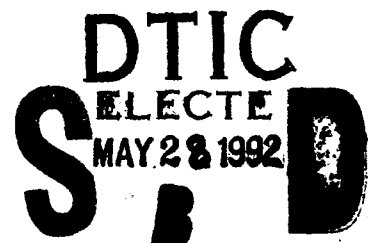

U.S. Army Laboratory Command
Harry Diamond Laboratories
Adelphi, MD 20783-1197

Approved for public release; distribution unlimited.

92-13998



92 5 27 071

The findings in this report are not to be construed as an official Department of the Army position unless so designated by other authorized documents.

Citation of manufacturer's or trade names does not constitute an official endorsement or approval of the use thereof.

Destroy this report when it is no longer needed. Do not return it to the originator.


REPORT DOCUMENTATION PAGE			Form Approved OMB No. 0704-0188	
Public reporting burden for this collection of information is estimated to average 1 hour per response, including the time for reviewing instructions, searching existing data sources, gathering and maintaining the data needed, and completing and reviewing the collection of information. Send comments regarding this burden estimate or any other aspect of this collection of information, including suggestions for reducing this burden, to Washington Headquarters Services, Directorate for Information Operations and Reports, 1215 Jefferson Davis Highway, Suite 1204, Arlington, VA 22202-4302, and to the Office of Management and Budget, Paperwork Reduction Project (0704-0188), Washington, DC 20503.				
1. AGENCY USE ONLY (Leave blank)		2. REPORT DATE April 1992		3. REPORT TYPE AND DATES COVERED Final, from 17 Oct 90 to 1 Feb 91
4. TITLE AND SUBTITLE Double-Sided Wafer Alignment Techniques			5. FUNDING NUMBERS PE: 62120	
6. AUTHOR(S) Timothy J. Mermagen and Bruce R. Geil				
7. PERFORMING ORGANIZATION NAME(S) AND ADDRESS(ES) Harry Diamond Laboratories 2800 Powder Mill Road Adelphi, MD 20783-1197			8. PERFORMING ORGANIZATION REPORT NUMBER	
9. SPONSORING/MONITORING AGENCY NAME(S) AND ADDRESS(ES) Naval Surface Warfare Center Dahlgren Laboratory Dahlgren, VA 22448			10. SPONSORING/MONITORING AGENCY REPORT NUMBER	
11. SUPPLEMENTARY NOTES AMS code: 612120.H250000 HDL PR: 122523				
12a. DISTRIBUTION/AVAILABILITY STATEMENT Approved for public release; distribution unlimited.			12b. DISTRIBUTION CODE	
13. ABSTRACT (Maximum 200 words) A project was undertaken by the Harry Diamond Laboratories to develop a double-sided wafer alignment technique by which special-purpose devices could be fabricated using in-house equipment. The approach developed was inexpensive and did not require infrared alignment methods for viewing through the wafer. A double-sided alignment technique with two different accuracies was developed for use on an ordinary optical mask aligner. These methods were highly successful and are in active use today.				
14. SUBJECT TERMS Double-sided wafer alignment, double polished wafers, optical mask aligner			15. NUMBER OF PAGES 14	
			16. PRICE CODE	
17. SECURITY CLASSIFICATION OF REPORT Unclassified	18. SECURITY CLASSIFICATION OF THIS PAGE Unclassified	17. SECURITY CLASSIFICATION OF ABSTRACT Unclassified	20. LIMITATION OF ABSTRACT UL	

Contents

	Page
1. Introduction	5
2. Alignment Technique	6
2.1 Lower Alignment Accuracy Technique	6
2.2 Higher Alignment Accuracy Technique	8
3. Results	12
4. Conclusions	12
Acknowledgements	12
Distribution	13

Figures

1. Lower accuracy alignment technique	7
2. Alignment windows	8
3. Semiconductor ignitor chip	8
4. Higher accuracy alignment technique	9
5. Edge alignment window with symbol bar	10
6. Scanning electron microscope photographs of cantilever beam accelerometer	11



Accession For	
NTIS GRA&I	☒
DTIC TAB	☐
Unannounced	☐
Justification	
By	
Distribution/	
Availability Codes	
Dist	Avail and/or Special
A-1	

1. Introduction

Front-to-back wafer alignment has been a problem for the semiconductor industry because of the cost and limited availability of the specialized equipment needed to easily perform this task. The user of an optical contact printer cannot see through the wafer to align the pattern on the front of the wafer to that on the back, as is possible with an infrared contact printer. In optical contact printing, therefore, problems with wafer rotation and displacement arise when the front and back patterns must be aligned. To solve these problems, a mask alignment technique has been designed in the Semiconductor Engineering and Materials Technology (SEMT) Facility of the Harry Diamond Laboratories (HDL). This technique allows the user to contact print quickly with a front-to-back alignment accuracy of better than 50 μm without the use of expensive through-the-wafer alignment equipment.

Two separate projects required accurately aligned photolithography on both sides of double-polished silicon wafers. The first project was fabrication of a chip for an in-house research program.¹ The second was fabrication of floating cantilever beams to be used as accelerometer switches.² The technique developed for aligning the patterns on the front and back of a wafer for these projects is described in this report.

¹Judith McCullen, Robert B. Reams, and Jonathan M. Terrell, *Failure Analysis of Loaded SCI Primers*, Harry Diamond Laboratories, HDL-PR-91-3 (September 1991).

²Theodore V. Blomquist and Timothy J. Mermagen, *Fabrication Process for Cantilever Beam Type Micromechanical Switch*, in preparation.

2. Alignment Technique

The alignment technique developed at HDL was devised for use with a one-to-one (no reduction) mask aligner. This technique was used with two alignment accuracies for the projects mentioned above; variations of this technique can also be used to pattern integrated circuits.

2.1 Lower Alignment Accuracy Technique


In the lower accuracy technique, the sides and flat of the wafer are used for aligning a mask to a wafer on a one-to-one mask aligner; figure 1a shows the mask used for this alignment accuracy. The mask consists of the first-level pattern with inter-level alignment marks (for same-side mask alignment) and the wafer edge windows. A *window* is an area where the chrome surface of a photomask has been removed, leaving the glass substrate uncovered. This allows for through-the-mask viewing.

Window C is used to align the flat of the wafer (fig. 1b and 2a). The user aligns the flat to the 500- μm bar separating the two 1000- μm -wide alignment windows. The lower part of window C is used to help find the flat of the wafer when higher magnifications are used. The user then aligns the flat as well as possible. When the back side of the wafer is imaged, this flat alignment will correct for rotational problems and correct for y -axis shift.

Once the flat of the wafer is aligned, the next step is the alignment of the wafer edge. Windows A and B are used for aligning the right or left edge of the wafer. These large windows contain a 100- μm bar that is used for aligning the wafer edge (see fig. 1c and 2b). Whichever edge/window is selected for alignment, the opposite edge/window must be used when the back of the wafer is aligned. This allows the die spacing to originate from the same side of the wafer, so that the front and back patterns on the wafer are aligned.

This alignment scheme produces better than 50- μm accuracy. This technique was successfully used to produce over 4000 test chips for an in-house research program (see fig. 3).

Figure 1. Lower accuracy alignment technique (a) mask, (b) flat alignment window, and (c) edge alignment window.

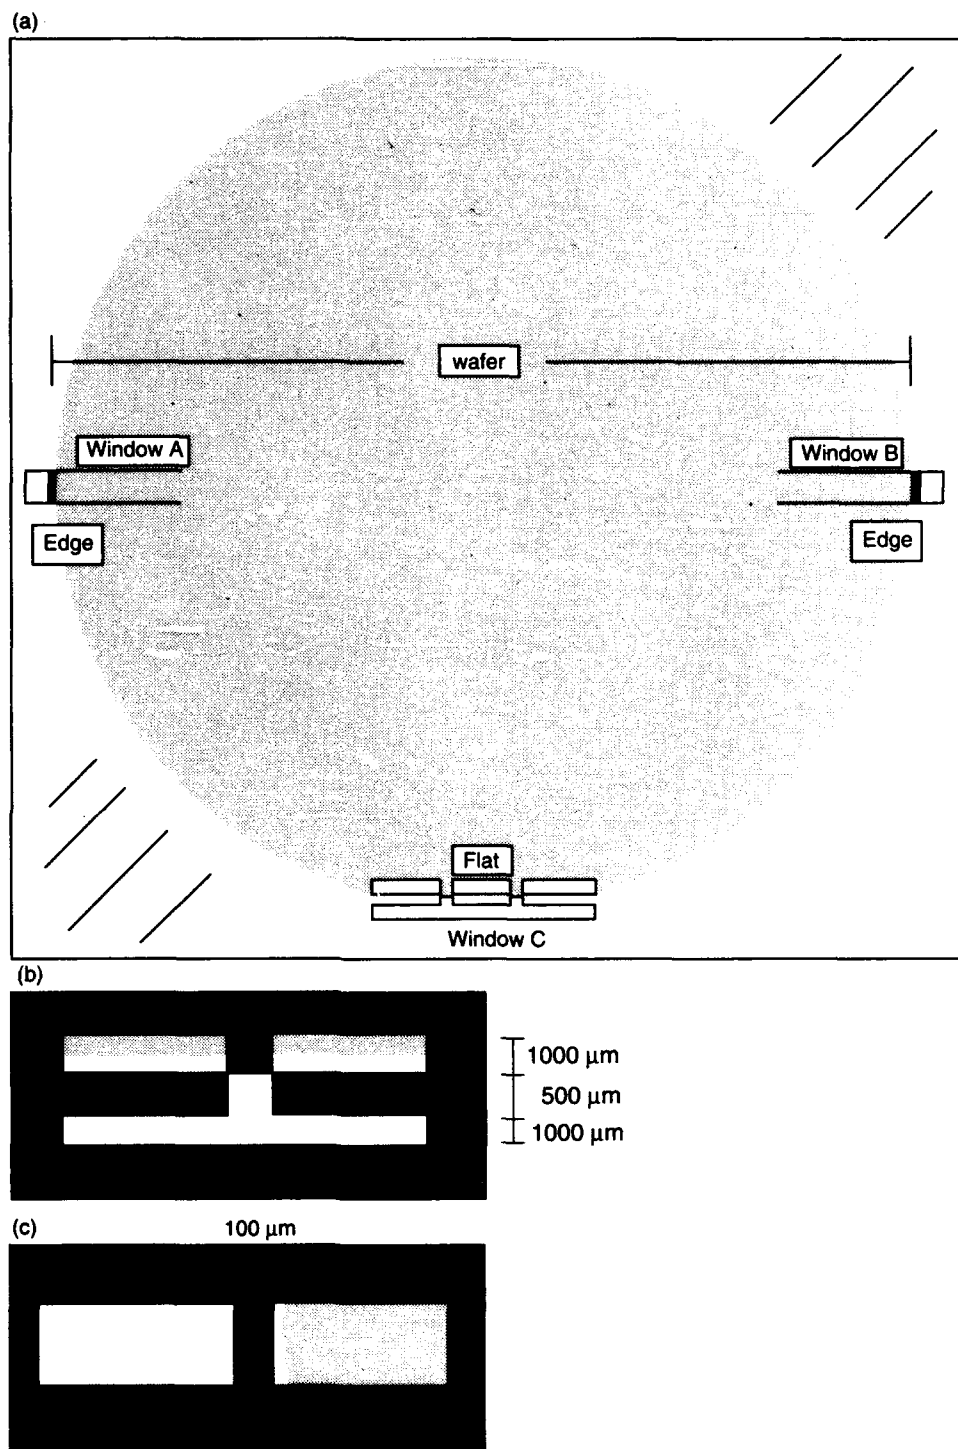

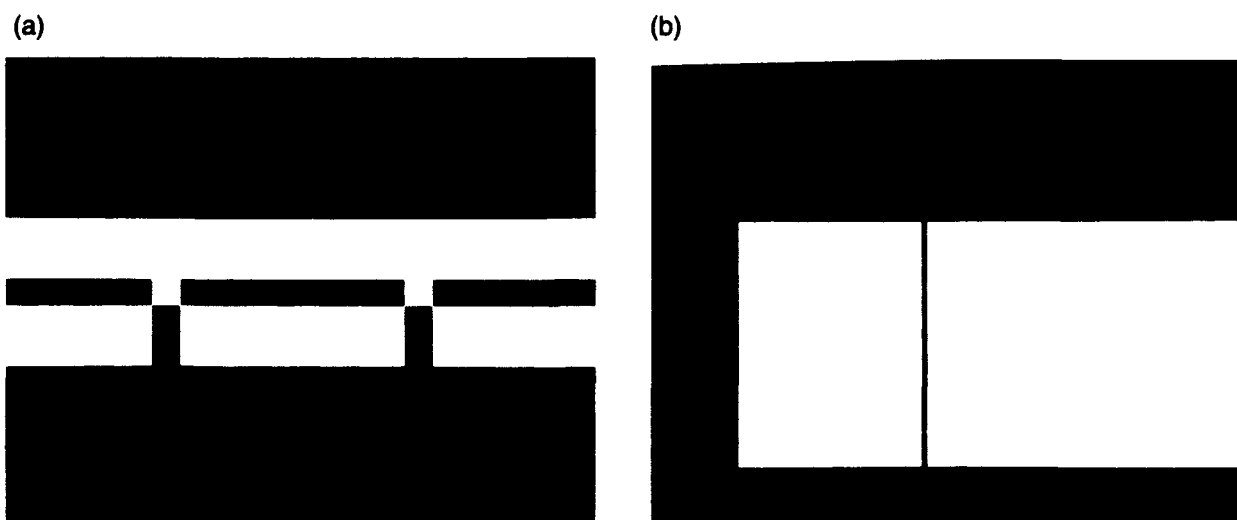


Figure 2. Alignment windows: (a) flat and (b) edge alignment window with 100- μm bar.

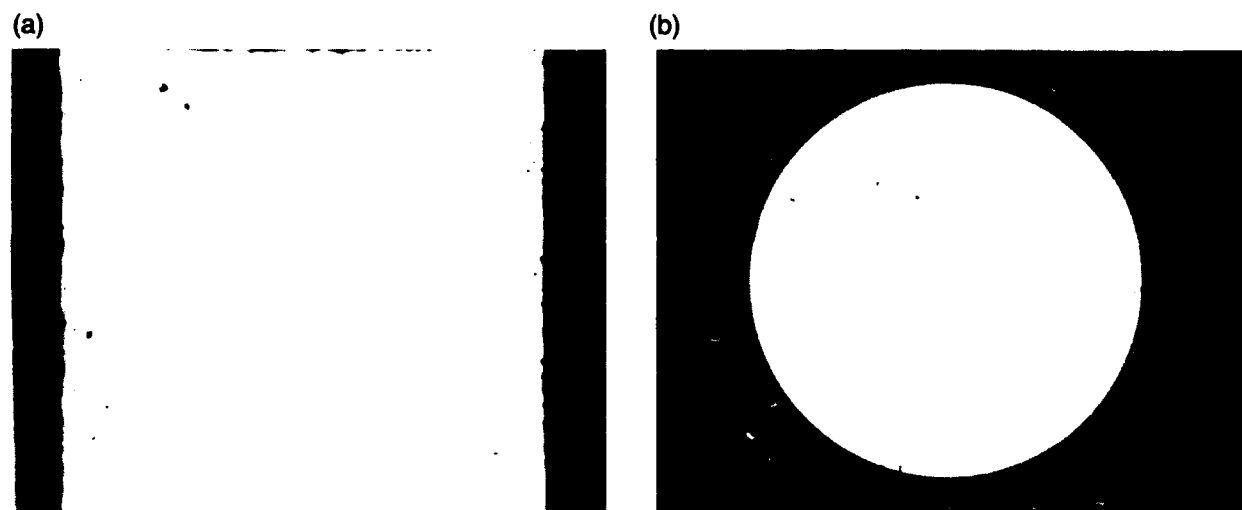





Figure 3. Semiconductor ignitor chip: (a) front view and (b) back view.

2.2 Higher Alignment Accuracy Technique

The second alignment technique also uses the sides and flat of the wafer to align a mask set on a one-to-one mask aligner, but it provides much higher accuracy (25 μm) and is much more difficult and time consuming to use. This mask alignment technique was used in the fabrication of floating cantilever beams.

The mask used in this technique has similar alignment windows to the previously described alignment mask. Window C is used in the same manner as in the first alignment mask: for aligning the flat of the wafer to correct for image rotation; it also aligns the wafer in the y -axis (fig. 4a and 4b). Again, once the flat is aligned, the wafer edge alignment is performed.

Figure 4. Higher accuracy alignment technique: (a) mask, (b) flat alignment window, and (c) edge alignment window.

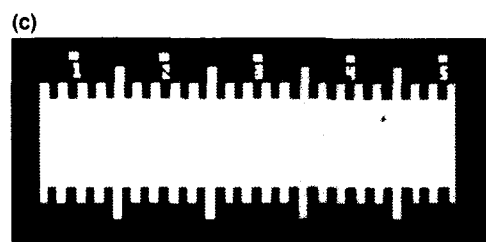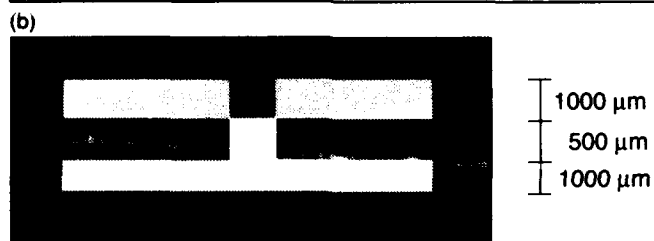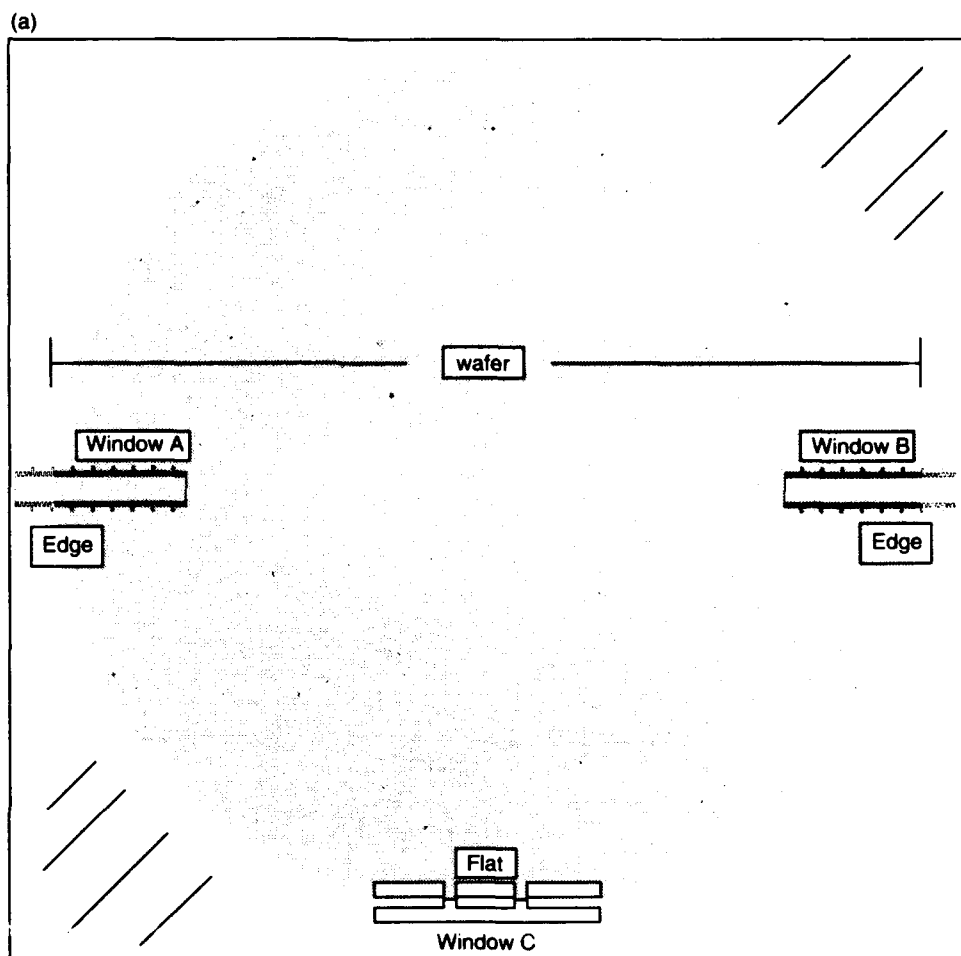

This alignment scheme produces better than 25- μm accuracy from front to back of the wafer. Several hundred cantilever accelerometers were produced using this method (see fig. 6).

Figure 1 consists of two panels, (a) and (b), each showing a bar chart of the number of correct responses (Y-axis, 0 to 100) versus the number of trials (X-axis, 1 to 10). Panel (a) shows a significant decrease in correct responses for the 100% condition (black bars) compared to the 50% condition (white bars). Panel (b) shows no significant difference between the 100% and 50% conditions.

Figure 6. Scanning electron microscope photographs of cantilever beam accelerometer: (a) top view and (b) side view.



3. Results

The results obtained with these alignment techniques have been very promising. With these techniques, we have produced over 4000 chips in support of the in-house research program and over 200 cantilever beam accelerometers. We have achieved a front-to-back wafer alignment accuracy of better than 50 μm with the lower accuracy technique and 25 μm with the higher accuracy technique on an ordinary optical contact printer.

4. Conclusions

The alignment techniques discussed here were very successful in aligning patterns on the top and back of a wafer and were used in producing chips and cantilever beam accelerometers. These techniques allow an inexpensive optical mask aligner system to be used to achieve much the same results as a more expensive infrared mask aligner.

Acknowledgements

The authors wish to acknowledge the assistance of two people in the work reported herein: Bernard Rod, HDL, for his work on the cantilever beam accelerometers; and Judith McCullen, HDL, for her untiring feedback on the alignment strategies and optical tooling of the in-house test chips and the cantilever beam accelerometer chips. The authors would also want to thank the rest of the Semiconductor Engineering and Materials Technology group for their support in this program.

Distribution

Administrator
Defense Technical Information Center
Attn DTIC-DDA (2 copies)
Cameron Station, Building 5
Alexandria, VA 22304-6145

Under Secretary of Defense for Research
& Engineering
Attn Research & Advanced Tech
Attn Asst to Sec/Atomic Energy
Attn Dep Asst Sec/Energy Environment & Safety
Attn Dep Under Sec/Res & Advanced Tech
Attn Dep Under Sec/Test & Evaluation
Department of Defense
Washington, DC 20301

Commander
CECOM R&D Tech Library
Attn ASQNC-ELC-IS-L-R
FT Monmouth, NJ 07703-5018

Director
US Army Ballistic Research Laboratory
Attn SLCBR
Attn SLCBR-AM
Attn SLCBR-X
Attn SLCBR-TB-VL
Aberdeen Proving Ground, MD 21005-5066

Director
US Army Electronic Warfare Laboratory,
LABCOM
Attn SLCET-D, Electronic Technology
& Devices Lab
Attn ASQNC-ELC-IS, Information Services
Div
FT Monmouth, NJ 07703-5601

Director
US Army Electronics Technology & Devices
Lab, LABCOM
Attn SLCET-E
Attn SLCET-ER
Attn SLCET-ER-S
Attn SLCET-I, Microelectronics
Attn SLCET-IA
FT Monmouth, NJ 07703-5601

Commander
US Army Materiel Command
Attn AMCDE, Dir for Dev & Engr
Attn AMCDE-R, Sys Eval & Testing
Attn AMCNC, Nuclear-Chemical Ofc
5001 Eisenhower Ave
Alexandria, VA 22333-0001

Director
Naval Research Laboratory
Attn Code 2620, Tech Library Br
Washington, DC 20375

Commander
Naval Surface Weapons Center
Attn Code WA501, Navy Nuc Prgms Ofc
Attn Code WA52
Attn Microelectronics, R. Goetz
Attn E-43, Technical Library
Attn WA50
White Oak, MD 20910

Commander
Naval Surface Weapons Center
Attn Code WR, Research & Technology Dept
Attn DX-21 Library Div
Attn H22, J. Bean
Attn H22, Richard Porter
Dahlgren Laboratory
Dahlgren, VA 22448

Distribution (cont'd)

Booz Allen & Hamilton, Inc.
Attn J. Terrell
4330 East-West Highway
Bethesda, MD 20814

US Army Laboratory Command
Attn AMSLC-DL, Dir, Corporate Labs

Installation Support Activity
Attn SLCIS-CC, Legal Office

USAISC
Attn AMSLC-IM-VA, Admin Ser Br
Attn AMSLC-IM-VP, Tech Pub Br
(2 copies)

Harry Diamond Laboratories
Attn Laboratory Directors
Attn SLCHD-TL, Library (3 copies)
Attn SLCHD-TL, Library (Woodbridge)
Attn SLCHD-NW, Deputy Director
Attn SLCHD-NW, J. M. McGarrity
Attn SLCHD-NW-CS, Chief
Attn SLCHD-NW-E, Chief
Attn SLCHD-NW-EH, Chief
Attn SLCHD-NW-EP, Chief
Attn SLCHD-NW-ES, Chief
Attn SLCHD-NW-P, Chief
Attn SLCHD-NW-RP, Chief

Harry Diamond Laboratories (cont'd)
Attn SLCHD-NW-RS, Chief
Attn SLCHD-NW-TN, Chief
Attn SLCHD-NW-TS, Chief
Attn SLCHD-D, R. Gilbert
Attn SLCHD-NW-EP, J. R. Miletta
Attn SLCHD-NW-P, D. Davis
Attn SLCHD-NW-RP, J. Benedetto
Attn SLCHD-NW-RP, K. W. Bennett
Attn SLCHD-NW-RP, T. V. Blomquist
Attn SLCHD-NW-RP, H. Boesch
Attn SLCHD-NW-RP, M. DeLancey
Attn SLCHD-NW-RP, T. Griffin
Attn SLCHD-NW-RP, A. J. Lelis
Attn SLCHD-NW-RP, B. McLean
Attn SLCHD-NW-RP, R. Moore
Attn SLCHD-NW-RP, T. Oldham
Attn SLCHD-NW-RP, C. Pennise
Attn SLCHD-NW-RP, R. B. Reams
Attn SLCHD-NW-RP, B. J. Rod
Attn SLCHD-NW-RP, T. Taylor
Attn SLCHD-NW-RS, H. Brandt
Attn SLCHD-NW-TS, H. Eisen
Attn SLCHD-TA-ES, R. Goodman
Attn SLCHD-NW-RP, J. McCullen
Attn SLCHD-NW-RP, B. Geil (10 copies)
Attn SLCHD-NW-RP, T. Mermagen
(15 copies)